
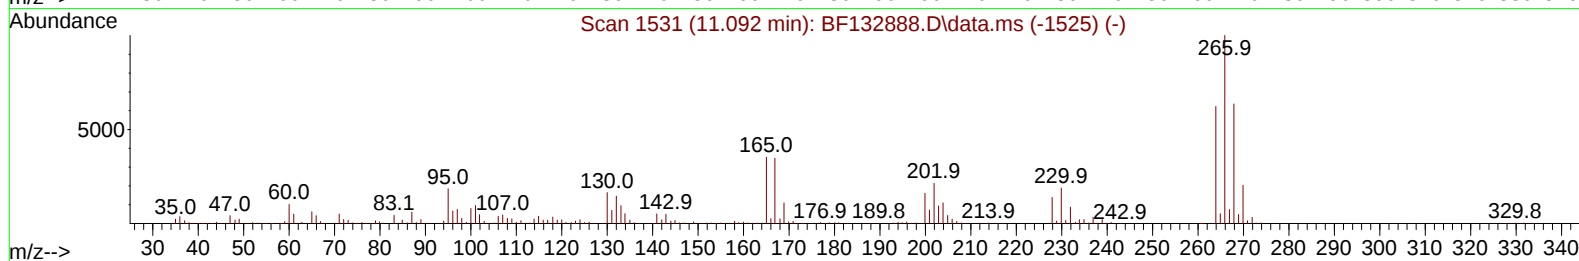
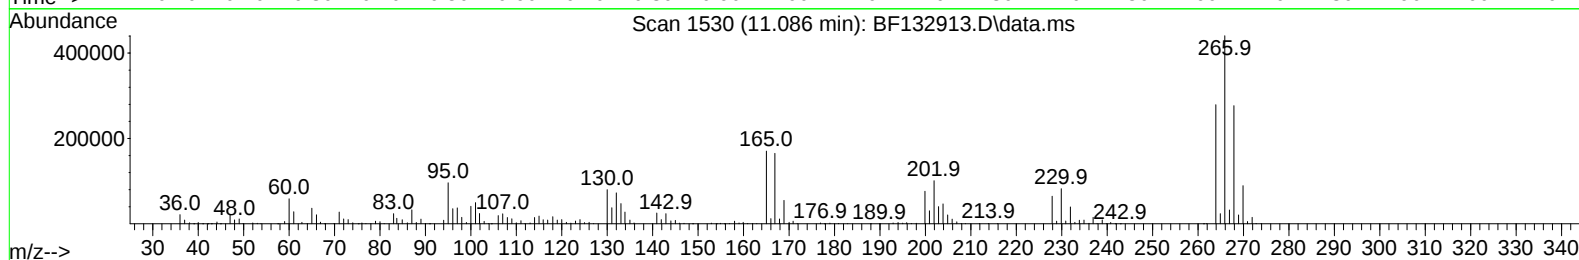


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041923\  
Data File : BF132913.D  
Acq On : 19 Apr 2023 15:53  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 05:08:02 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF041723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 18 04:51:21 2023  
Response via : Initial Calibration

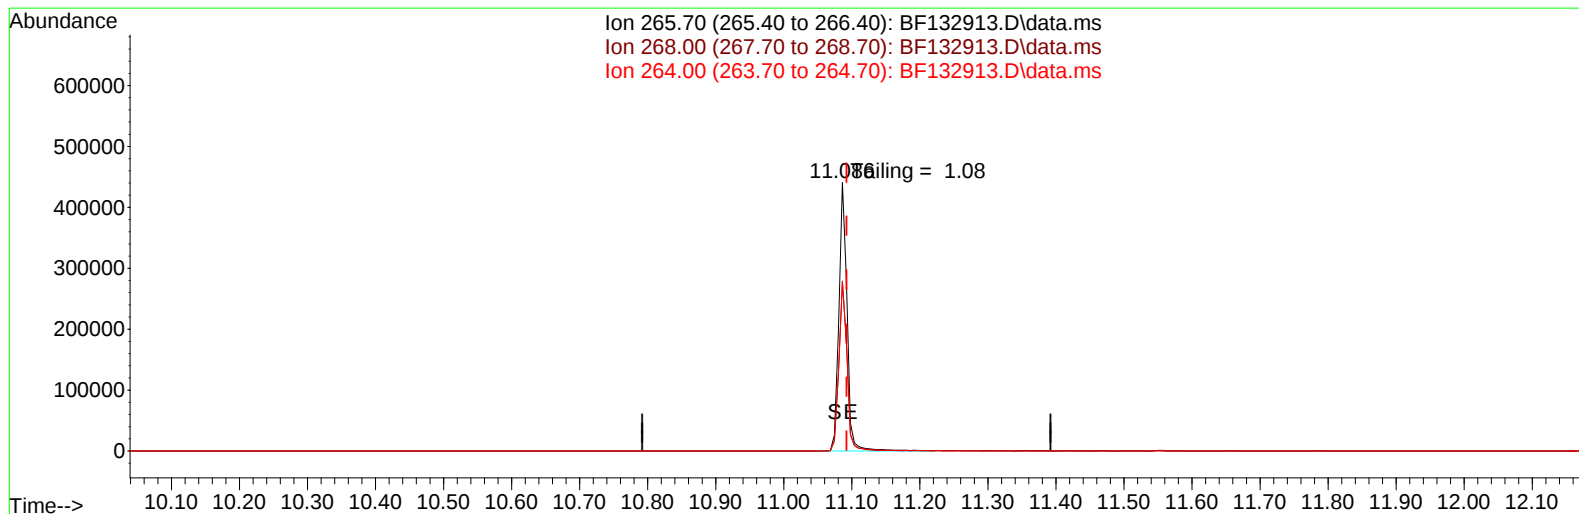

TIC: BF132913.D\data.ms

**(70) Pentachlorophenol (C)**




11.086min (-0.006) 330404.16 ng

response 366250

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.60  | 62.80  |
| 264.00 | 62.20  | 63.31  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041923\  
Data File : BF132913.D  
Acq On : 19 Apr 2023 15:53  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 05:16:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF041723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 18 04:51:21 2023  
Response via : Initial Calibration

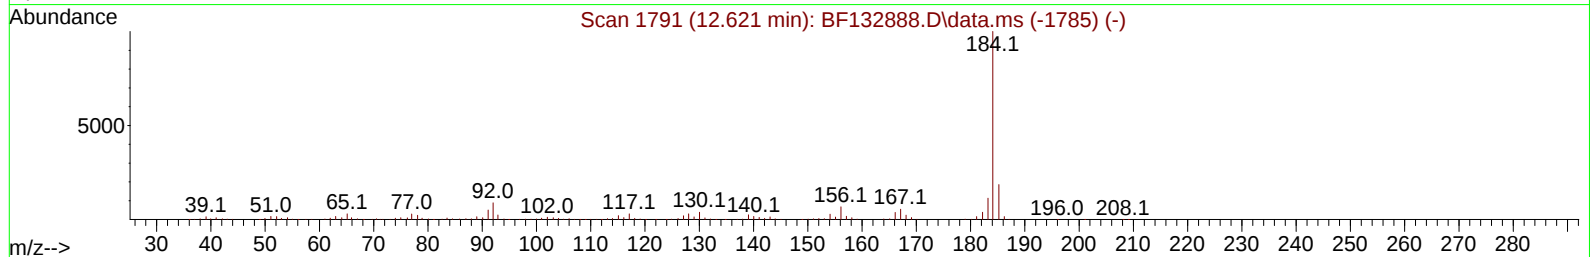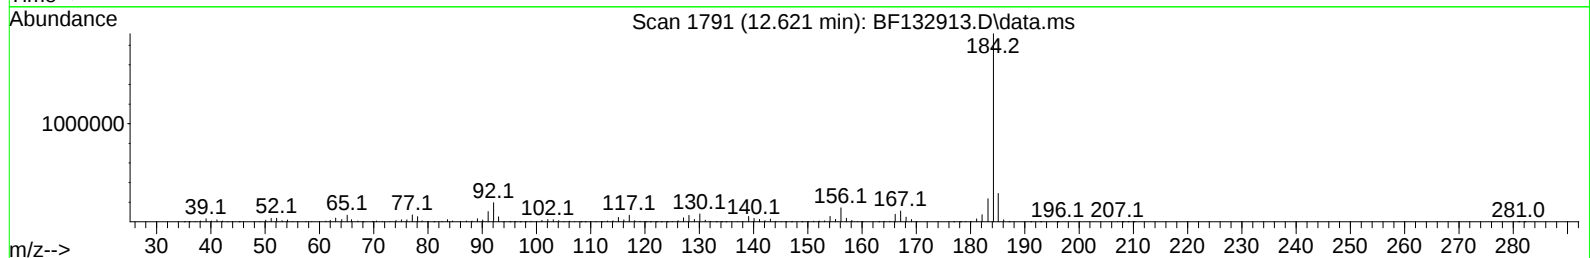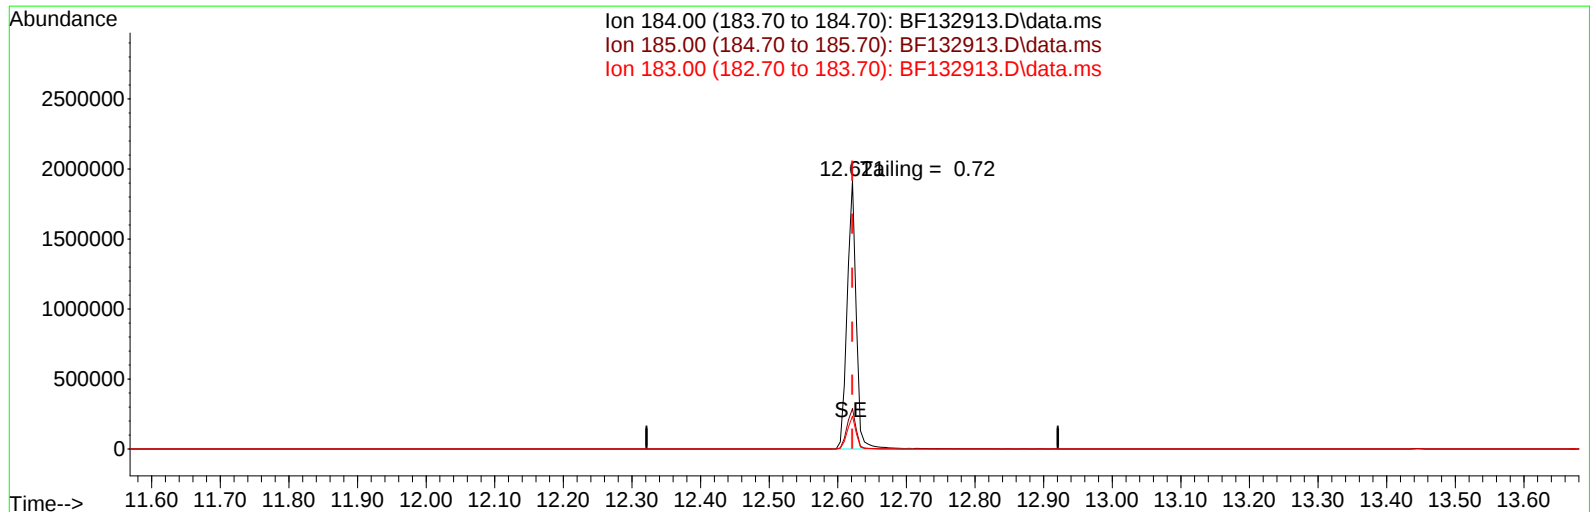

TIC: BF132913.D\data.ms

**(77) Benzidine**

12.621min (+ 0.000) 11425.98 ng

response 1749991

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 18.60  | 15.08  |
| 183.00 | 11.30  | 12.31  |
| 0.00   | 0.00   | 0.00   |