
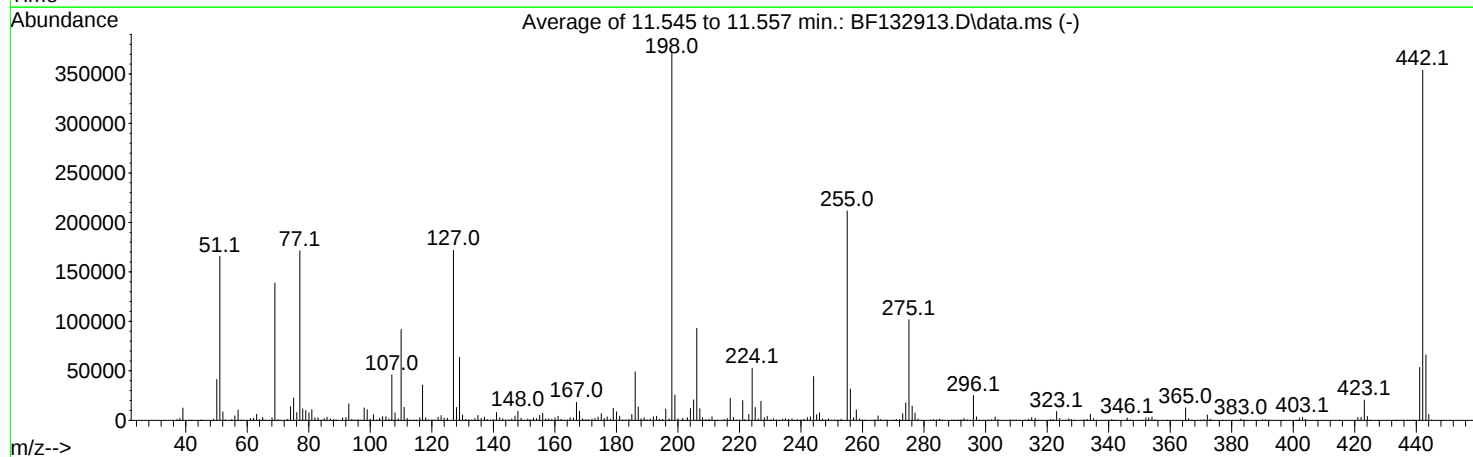


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041923\
Data File : BF132913.D
Acq On : 19 Apr 2023 15:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 20 14:15:37 2023

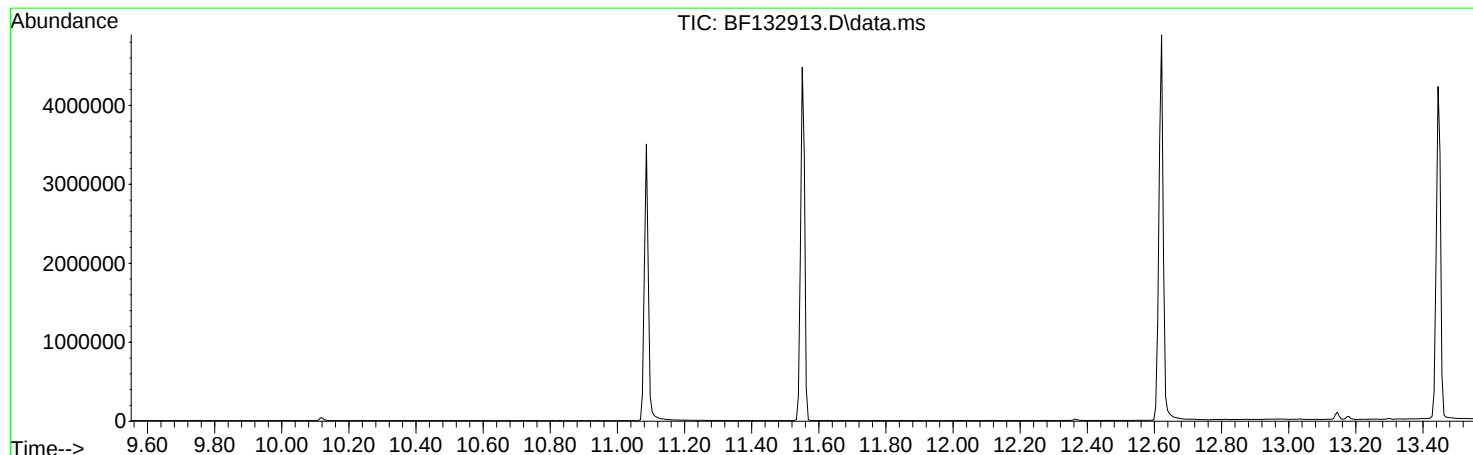




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	165627	PASS
68	69	0.00	2	1.9	2586	PASS
69	198	0.00	100	37.3	138675	PASS
70	69	0.00	2	0.5	687	PASS
127	198	10	80	46.2	171819	PASS
197	198	0.00	2	0.4	1543	PASS
198	198	100	100	100.0	371797	PASS
199	198	5	9	6.9	25699	PASS
275	198	10	60	27.4	101699	PASS
365	198	1	100	3.4	12511	PASS
441	198	0.01	100	14.4	53485	PASS
442	442	50	100	100.0	353803	PASS
443	442	15	24	18.7	66072	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041923\
Data File : BF132913.D
Acq On : 19 Apr 2023 15:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 20 05:08:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

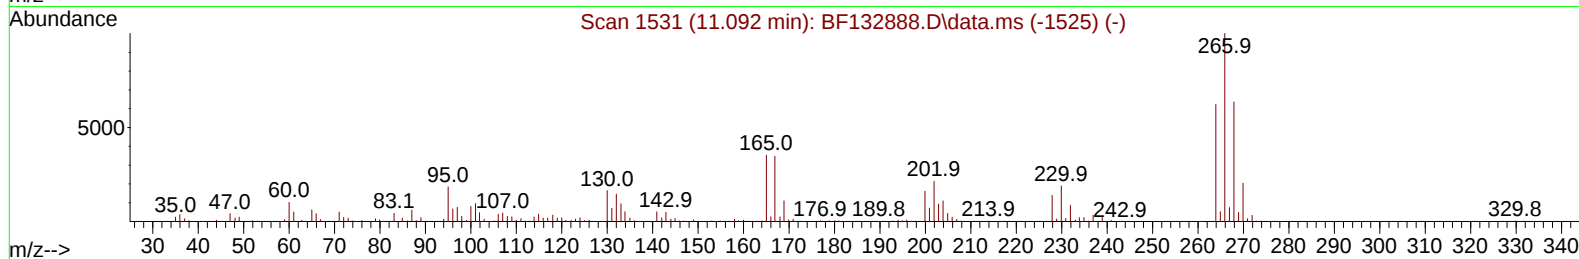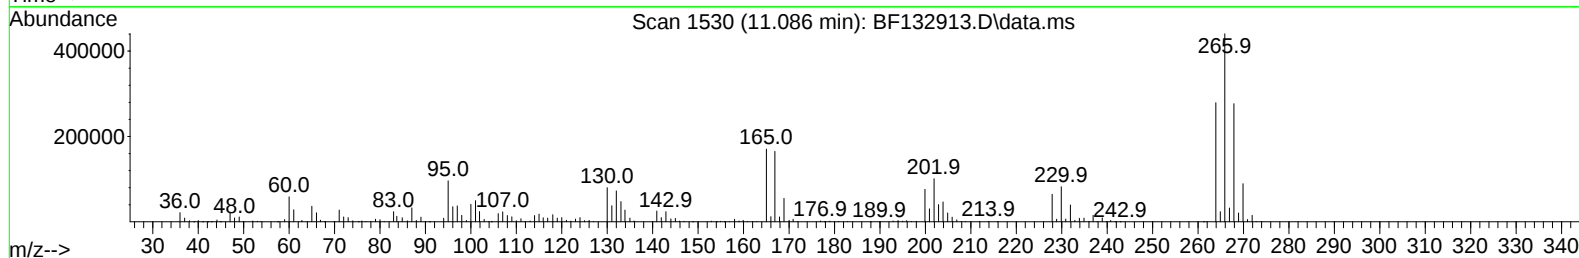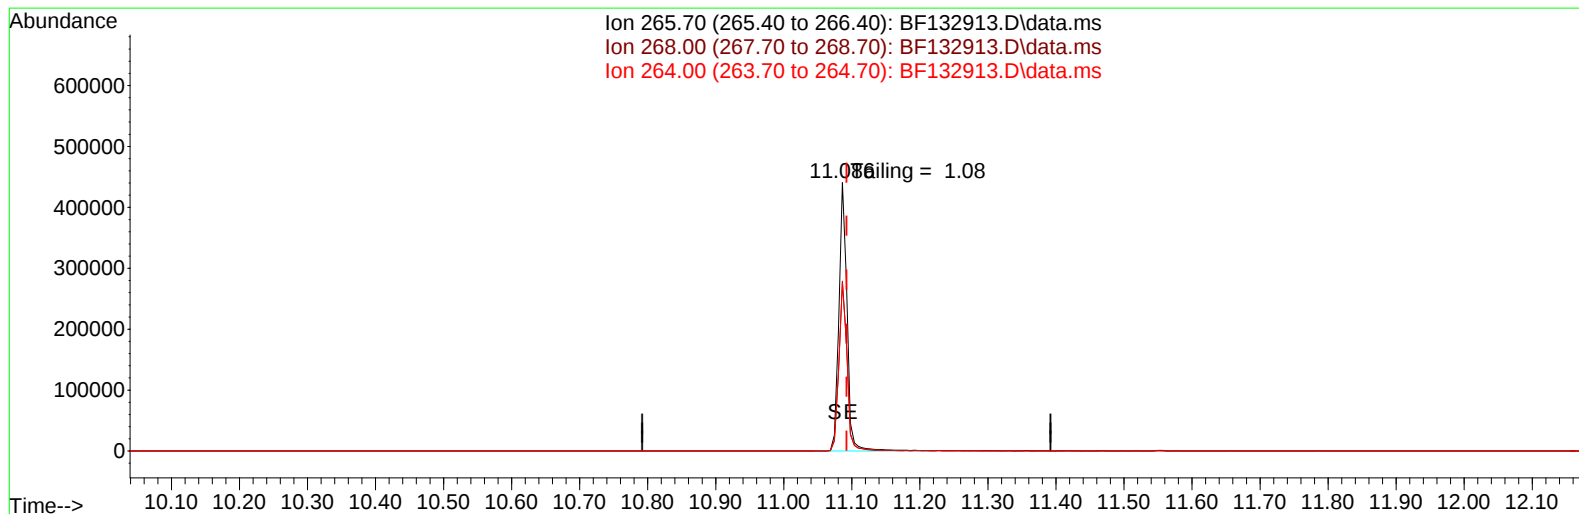

TIC: BF132913.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 330404.16 ng




response 366250

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.80
264.00	62.20	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041923\
 Data File : BF132913.D
 Acq On : 19 Apr 2023 15:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 20 05:16:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 04:51:21 2023
 Response via : Initial Calibration

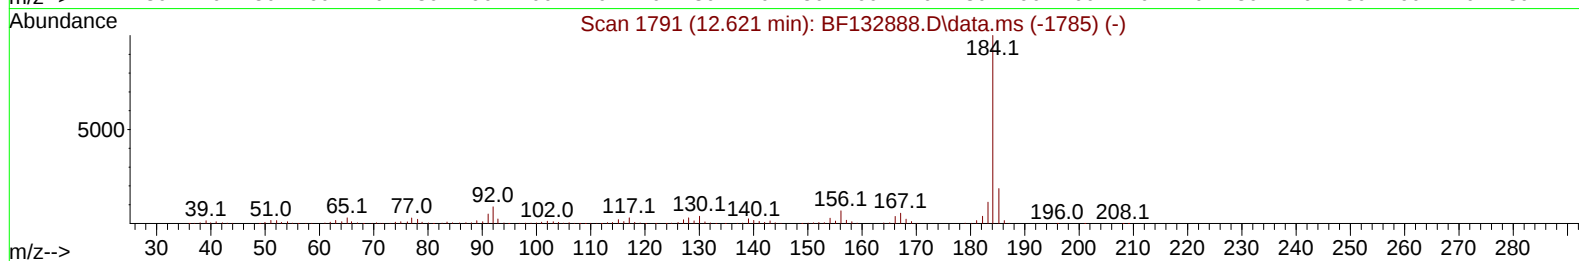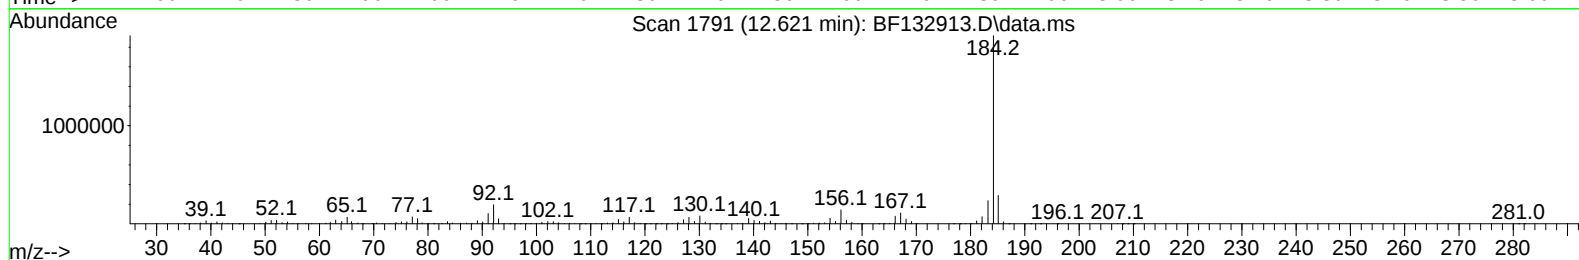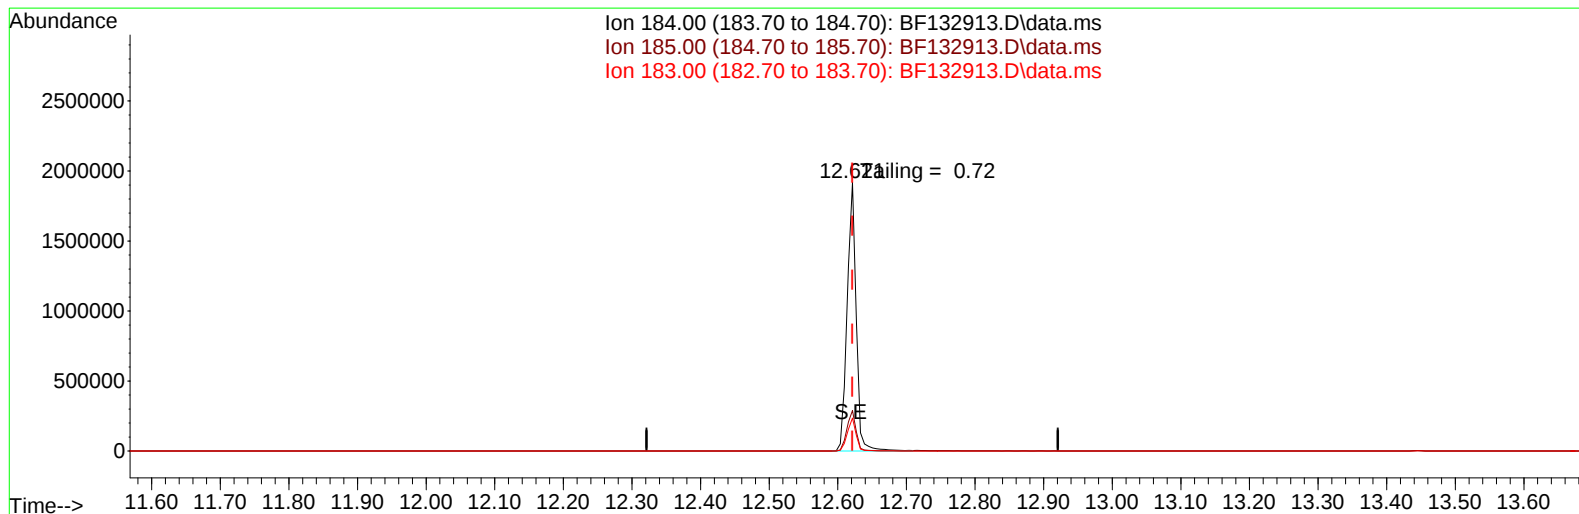

TIC: BF132913.D\data.ms

(77) Benzidine

12.621min (+ 0.000) 11425.98 ng

response 1749991

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	15.08
183.00	11.30	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2023	BNA_F	<u>BF132913.D</u>
Compound Name	Response	Retention Time
DDT	684172	13.445
DDD	19419	13.145
DDE	610	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20029	704201	2.84

Instrument :
BNA_F
ClientSampleId :
DFTPP