

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042020\
 Data File : BF120077.D
 Acq On : 20 Apr 2020 15:02
 Operator : MA/SJ
 Sample : L2242-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-1RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.322	545	550	553	rBV	2944332	2961084	78.65%	8.366%
2	6.357	720	726	729	rBV	2850157	3003623	79.78%	8.486%
3	6.551	756	759	767	rVB2	58414	65161	1.73%	0.184%
4	6.716	783	787	790	rBV	972625	867161	23.03%	2.450%
5	6.869	809	813	817	rBV	2778082	2491884	66.19%	7.040%
6	7.281	878	883	886	rBV	1941768	1807643	48.01%	5.107%
7	7.998	1001	1005	1009	rBV	1257173	1061518	28.20%	2.999%
8	9.080	1184	1189	1192	rBV	3912647	3368356	89.47%	9.516%
9	9.475	1252	1256	1259	rBV	615072	459237	12.20%	1.297%
10	9.757	1299	1304	1307	rBV	1603841	1294941	34.40%	3.658%
11	9.786	1307	1309	1313	rVB	64184	51066	1.36%	0.144%
12	9.963	1336	1339	1343	rBV	54076	47975	1.27%	0.136%
13	10.304	1394	1397	1402	rVB	121607	100528	2.67%	0.284%
14	10.551	1433	1439	1442	rBV	2035870	2055467	54.60%	5.807%
15	11.245	1553	1557	1559	rBV	1449521	1260763	33.49%	3.562%
16	11.263	1559	1560	1564	rVV	264513	209085	5.55%	0.591%
17	11.316	1564	1569	1573	rVB	64239	56682	1.51%	0.160%
18	11.745	1639	1642	1644	rBV	48082	41497	1.10%	0.117%
19	11.780	1644	1648	1653	rBV2	635836	607447	16.13%	1.716%
20	11.857	1658	1661	1663	rBV	105193	89888	2.39%	0.254%
21	11.951	1670	1677	1680	rBV6	53287	104265	2.77%	0.295%
22	12.063	1694	1696	1702	rVB4	42133	42035	1.12%	0.119%
23	12.457	1759	1763	1766	rBV	512127	435055	11.56%	1.229%
24	12.504	1769	1771	1777	rVB6	28840	38740	1.03%	0.109%
25	12.563	1777	1781	1786	rBV2	167735	210178	5.58%	0.594%
26	12.686	1796	1802	1804	rBV	388575	415096	11.03%	1.173%
27	12.839	1823	1828	1831	rVB	3964815	3764804	100.00%	10.636%
28	12.904	1835	1839	1843	rBV3	35871	55415	1.47%	0.157%
29	13.015	1855	1858	1861	rVB	80783	74481	1.98%	0.210%
30	13.051	1861	1864	1866	rBV4	36424	47190	1.25%	0.133%
31	13.080	1866	1869	1872	rVB2	78259	79549	2.11%	0.225%
32	13.115	1872	1875	1878	rBV	47655	46157	1.23%	0.130%
33	13.315	1906	1909	1915	rVB6	54847	63416	1.68%	0.179%
34	13.415	1921	1926	1928	rBV2	57583	63619	1.69%	0.180%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042020\
 Data File : BF120077.D
 Acq On : 20 Apr 2020 15:02
 Operator : MA/SJ
 Sample : L2242-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-1RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.633	1959	1963	1965	rBV2	38247	48654	1.29%	0.137%
36	13.739	1977	1981	1990	rVB	624760	771753	20.50%	2.180%
37	13.886	2000	2006	2008	rBV2	1306688	1299487	34.52%	3.671%
38	13.910	2008	2010	2013	rVB	202007	146591	3.89%	0.414%
39	14.062	2032	2036	2040	rBV2	89262	106573	2.83%	0.301%
40	14.368	2084	2088	2094	rBV3	171123	285543	7.58%	0.807%
41	14.639	2131	2134	2136	rBV	67597	72511	1.93%	0.205%
42	14.662	2136	2138	2144	rVB	113369	111284	2.96%	0.314%
43	14.898	2164	2178	2188	rVB2	417692	1636710	43.47%	4.624%
44	14.986	2189	2193	2195	rBV	129111	158657	4.21%	0.448%
45	15.186	2225	2227	2233	rVB	96908	110532	2.94%	0.312%
46	15.245	2234	2237	2243	rVB	134510	137302	3.65%	0.388%
47	15.309	2243	2248	2251	rBV	652544	793531	21.08%	2.242%
48	15.339	2251	2253	2258	rVV2	109733	138408	3.68%	0.391%
49	15.474	2262	2276	2290	rVB8	332482	1533540	40.73%	4.333%
50	15.756	2320	2324	2328	rVB	79113	108376	2.88%	0.306%
51	15.809	2329	2333	2341	rVV4	61746	130792	3.47%	0.370%
52	16.227	2401	2404	2410	rBV	36204	60748	1.61%	0.172%
53	16.503	2447	2451	2454	rBV5	36240	69560	1.85%	0.197%
54	16.686	2478	2482	2490	rVB3	100173	204478	5.43%	0.578%
55	17.103	2547	2553	2556	rBV2	64833	129519	3.44%	0.366%


Sum of corrected areas: 35395555

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042020\
Data File : BF120077.D
Acq On : 20 Apr 2020 15:02
Operator : MA/SJ
Sample : L2242-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-1RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

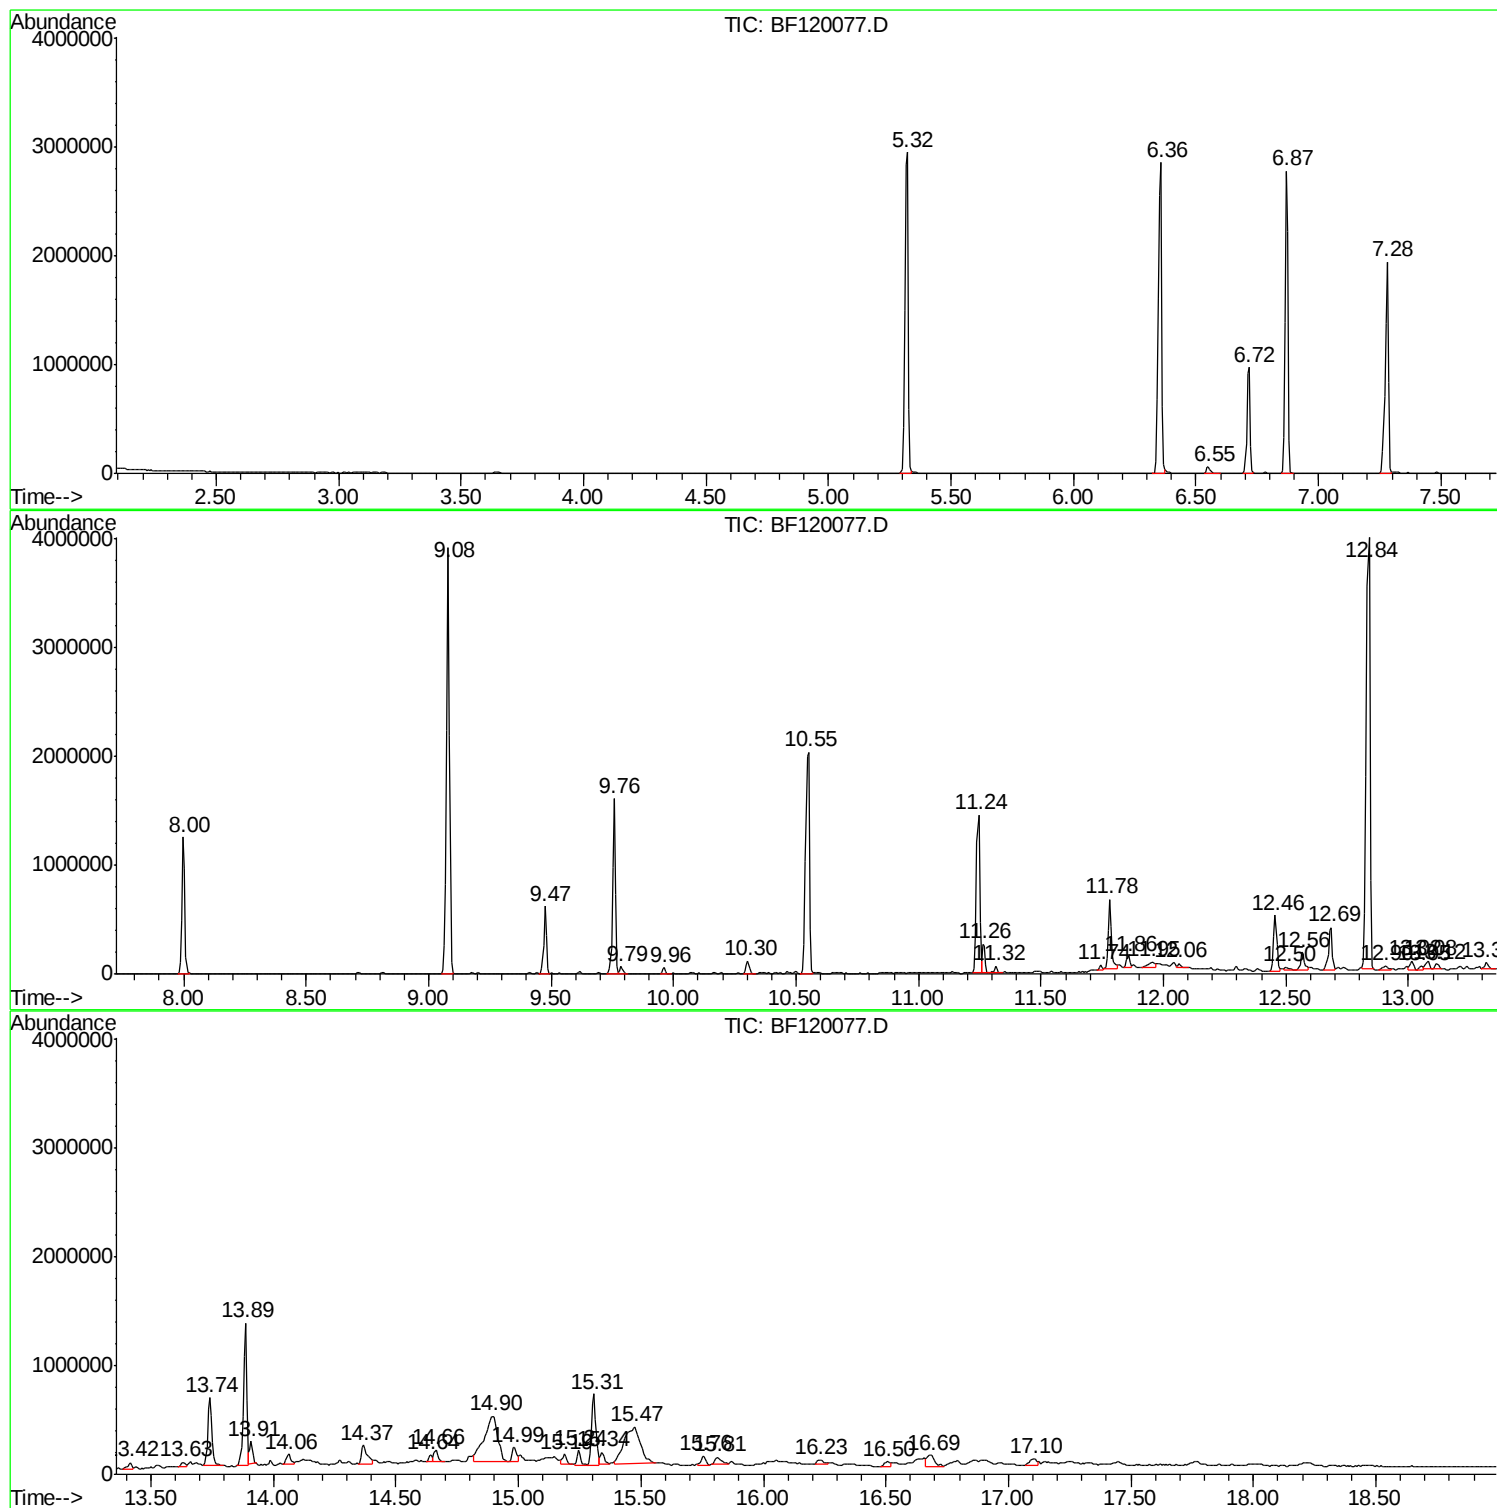

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042020\
Data_File : BF120077.D
Acq_On : 20 Apr 2020 15:022
Operator : MA/SJJ
Sample : L2242-01REE
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
B-1RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
