


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042020\
 Data File : BF120072.D
 Acq On : 20 Apr 2020 12:11
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 20 14:10:57 2020

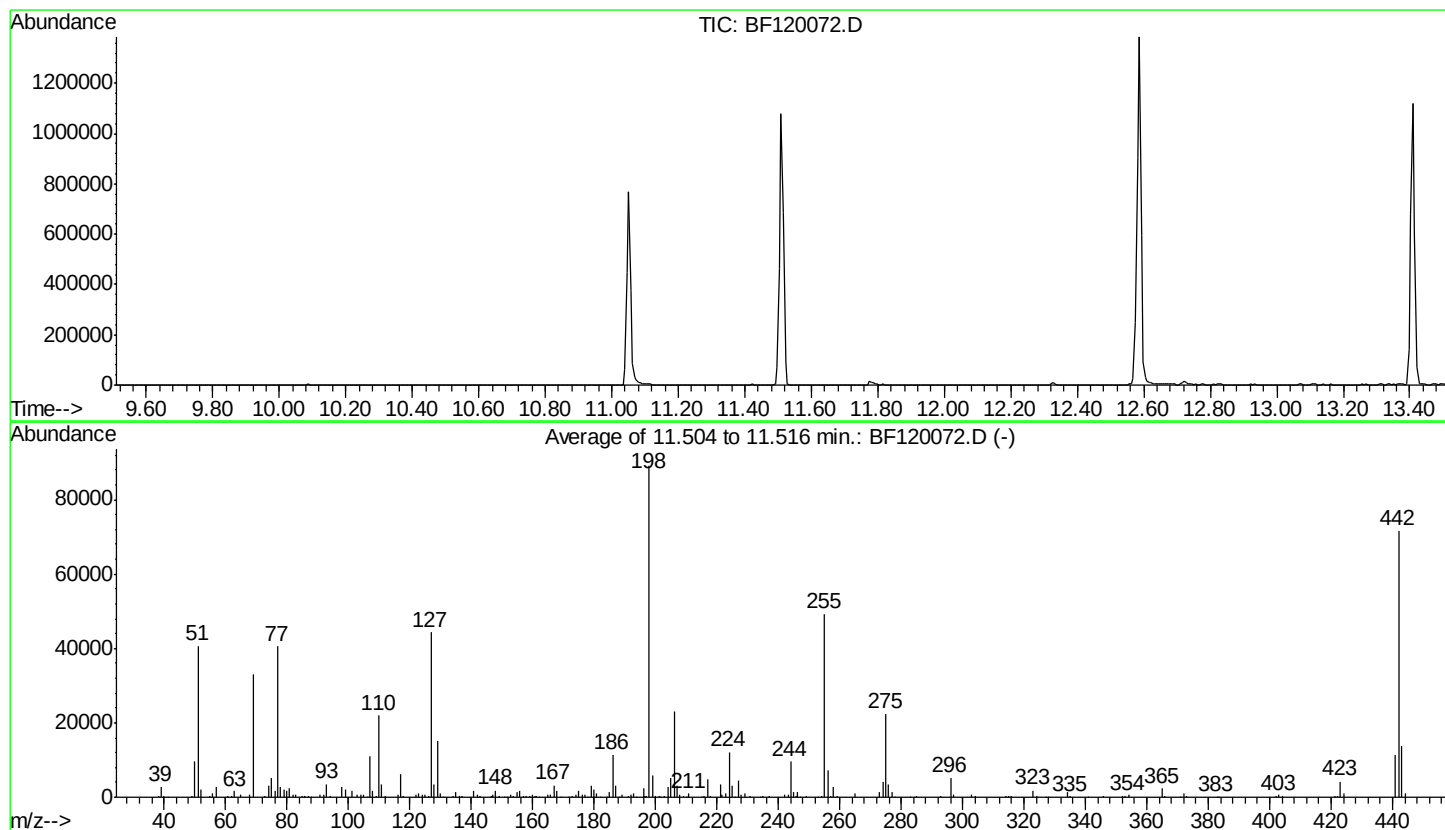

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	40738	PASS
68	69	0.00	2	1.8	607	PASS
69	198	0.00	100	37.0	32936	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	44301	PASS
197	198	0.00	2	0.5	441	PASS
198	198	100	100	100.0	89128	PASS
199	198	5	9	6.5	5768	PASS
275	198	10	60	25.1	22394	PASS
365	198	1	100	2.6	2286	PASS
441	198	0.01	100	12.7	11311	PASS
442	198	50	100	80.5	71709	PASS
443	442	15	24	19.1	13725	PASS