

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042120\
 Data File : BF120108.D
 Acq On : 21 Apr 2020 17:58
 Operator : MA/SJ
 Sample : L2343-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1B

Quant Time: Apr 22 03:16:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 21 13:48:22 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	126030	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	480568	20.00	ng	0.00
39) Acenaphthene-d10	9.73	164	233534	20.00	ng	0.00
64) Phenanthrene-d10	11.22	188	394142	20.00	ng	0.00
76) Chrysene-d12	13.86	240	238160	20.00	ng	0.00
87) Perylene-d12	15.29	264	252778	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	850374	116.61	ng	0.00
7) Phenol-d6	6.33	99	1088378	115.82	ng	0.00
23) Nitrobenzene-d5	7.26	82	702737	75.65	ng	0.00
42) 2,4,6-Tribromophenol	10.53	330	251532	87.97	ng	0.00
45) 2-Fluorobiphenyl	9.06	172	1295729	78.77	ng	0.00
79) Terphenyl-d14	12.81	244	1005527	71.04	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.45	163	208627	11.550	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042120\
Data File : BF120108.D
Acq On : 21 Apr 2020 17:58
Operator : MA/SJ
Sample : L2343-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1B

Quant Time: Apr 22 03:16:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 13:48:22 2020
Response via : Initial Calibration

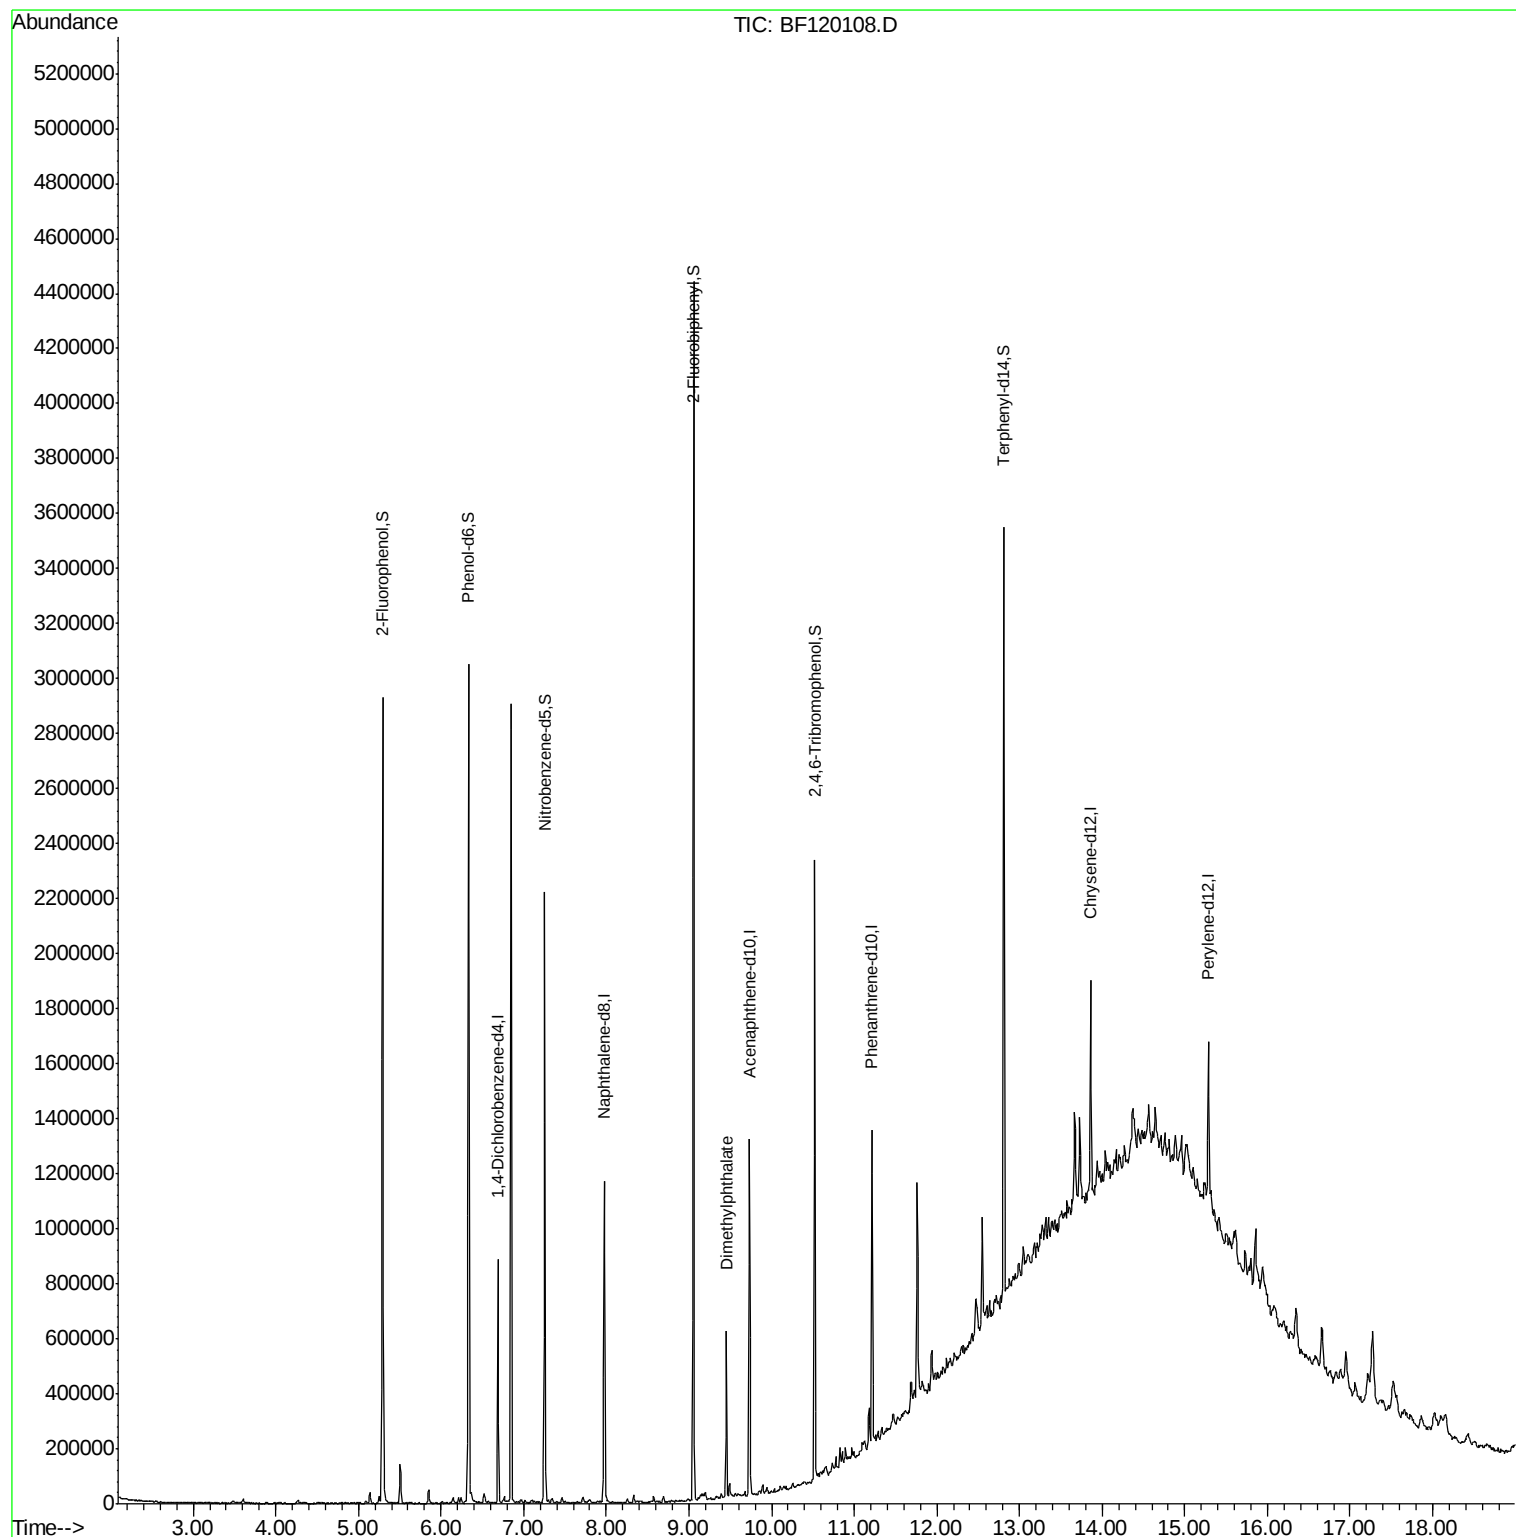

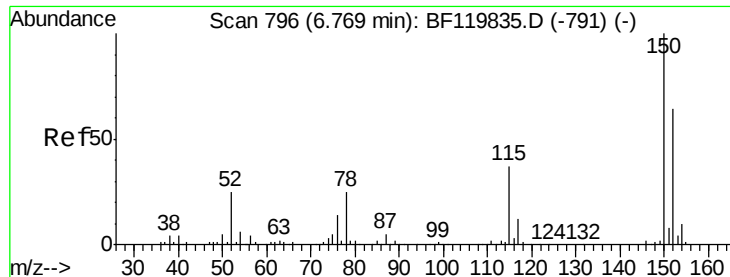


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.69 min Scan# 783
Delta R.T. -0.00 min
Lab File: BF120108.D
Acq: 21 Apr 2020 17:58

Instrument :
BNA_F
ClientSampleId :
SB-1B

Tot Ion:152 Resp: 126030
Ion Ratio Lower Upper
152 100
150 153.7 124.8 187.2
115 57.4 46.5 69.7

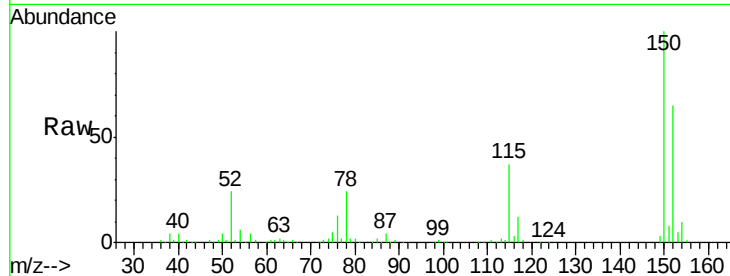


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

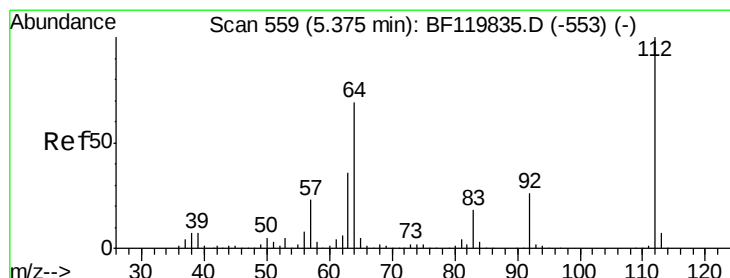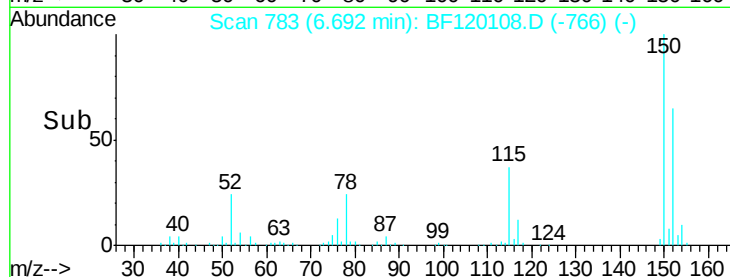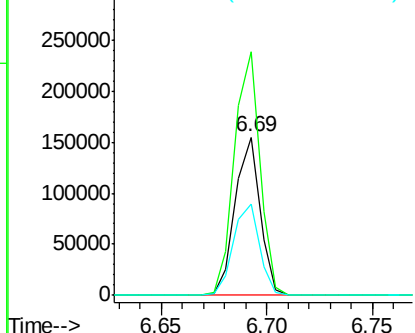



#5


2-Fluorophenol
Concen: 116.607 ng
RT: 5.30 min Scan# 546
Delta R.T. 0.01 min
Lab File: BF120108.D
Acq: 21 Apr 2020 17:58

Tgt Ion:112 Resp: 850374
Ion Ratio Lower Upper
112 100
64 64.4 55.5 83.3
63 33.4 29.1 43.7

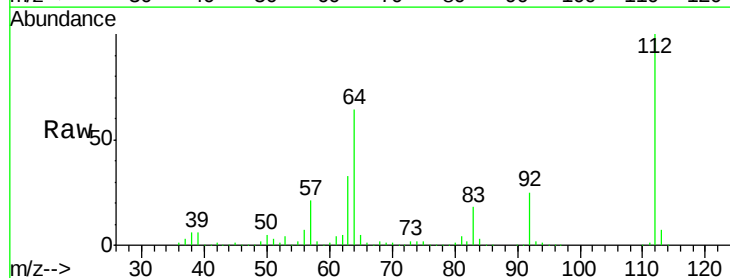

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

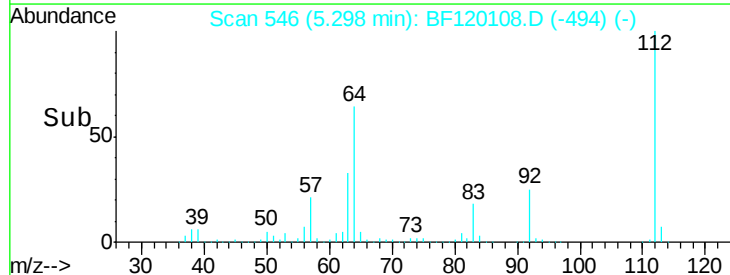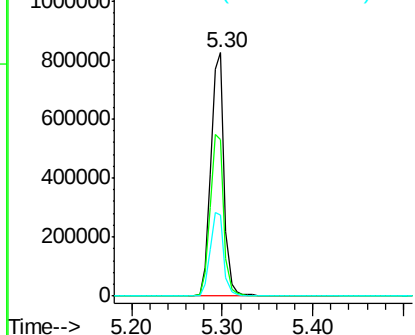

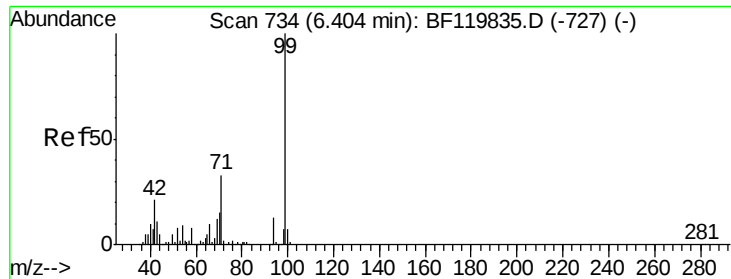

#7

Phenol-d6

Concen: 115.823 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.00 min

Lab File: BF120108.D

Acq: 21 Apr 2020 17:58

Instrument :

BNA_F

ClientSampled :

SB-1B


Tot Ion: 99 Resp: 1088378

Ion Ratio Lower Upper

99 100

42 20.7 16.9 25.3




71 33.0 26.3 39.5

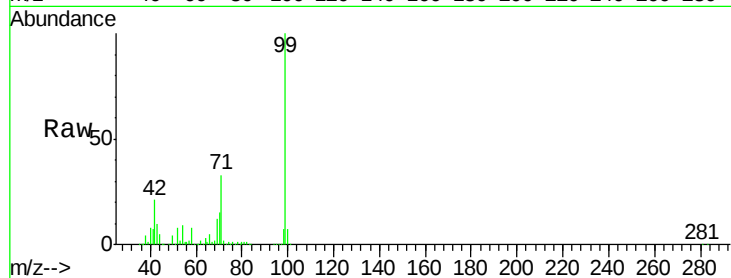

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

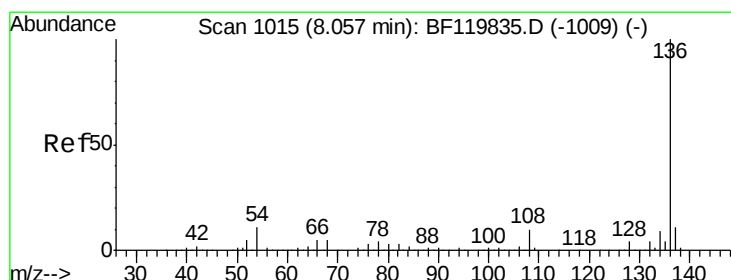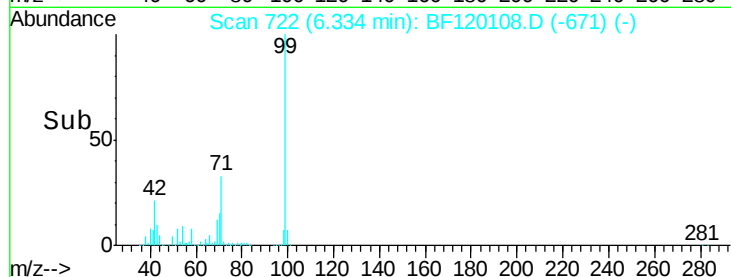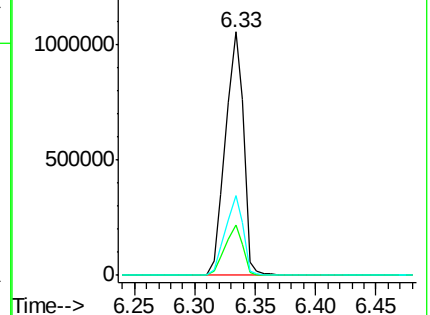

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1001

Delta R.T. -0.01 min

Lab File: BF120108.D

Acq: 21 Apr 2020 17:58

Tgt Ion: 136 Resp: 480568


Ion Ratio Lower Upper

136 100

137 11.5 8.7 13.1

54 10.3 8.5 12.7

68 5.6 3.9 5.9


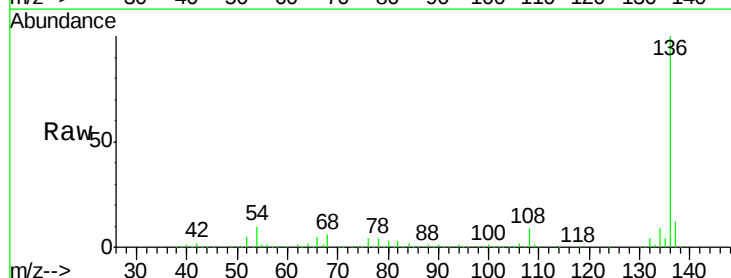



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



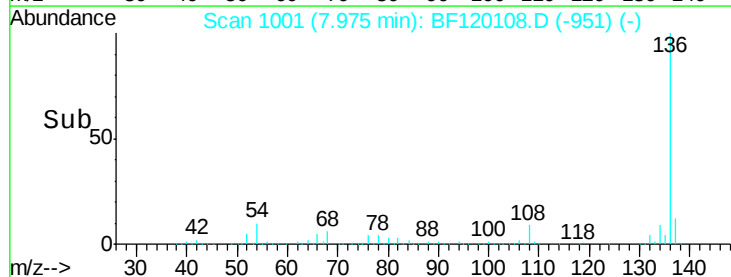
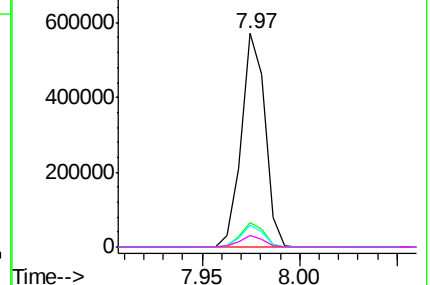


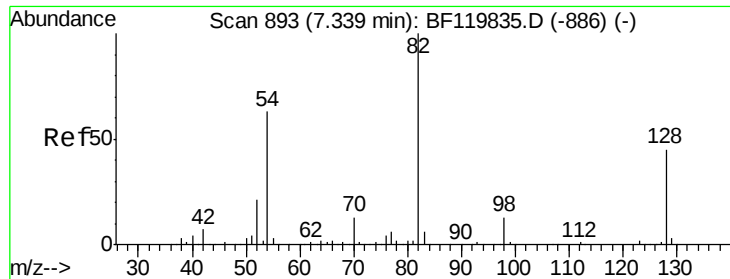

#23
Nitrobenzene-d5
Concen: 75.650 ng
RT: 7.26 min Scan# 879
Delta R.T. -0.01 min
Lab File: BF120108.D
Acq: 21 Apr 2020 17:58




Instrument :
BNA_F
ClientSampleId :
SB-1B


Tot Ion: 82 Resp: 702737
Ion Ratio Lower Upper
82 100
128 45.7 36.2 54.4
54 63.5 50.4 75.6

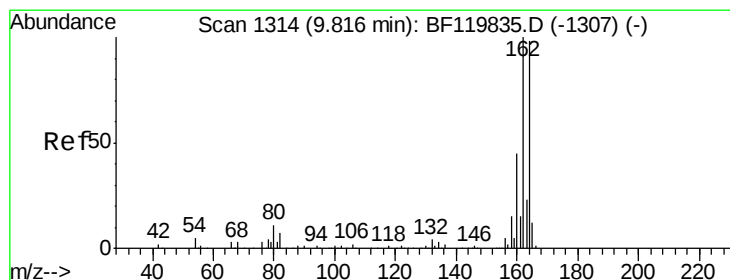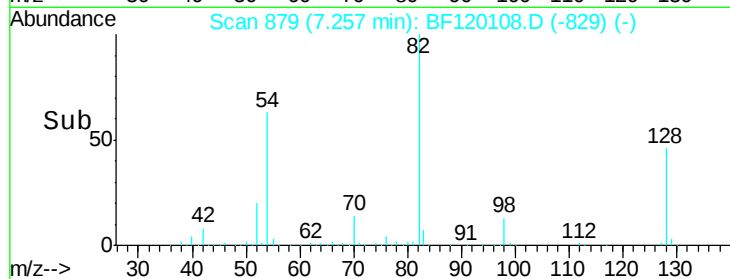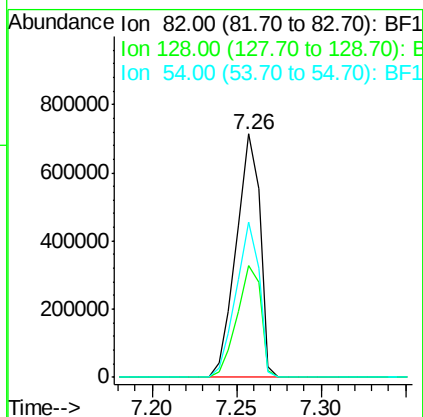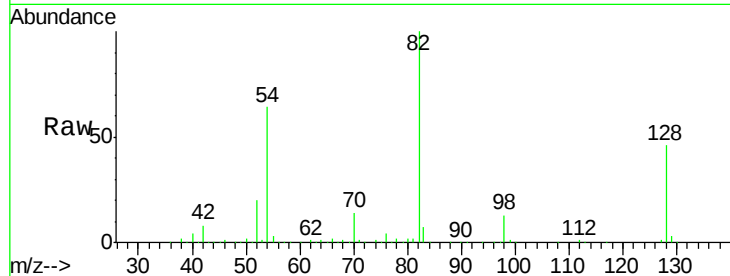

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.73 min Scan# 1300
Delta R.T. -0.01 min
Lab File: BF120108.D
Acq: 21 Apr 2020 17:58

Tgt Ion:164 Resp: 233534
Ion Ratio Lower Upper
164 100
162 104.3 81.9 122.9
160 46.0 36.6 54.8

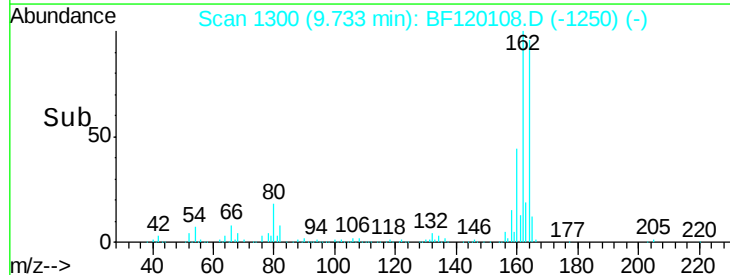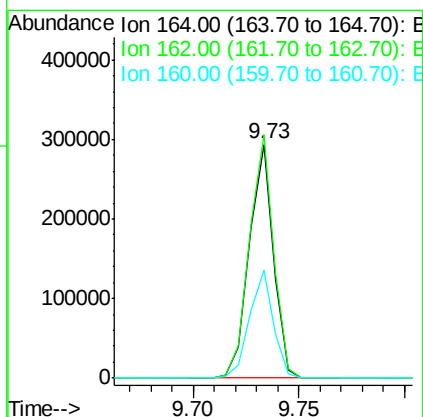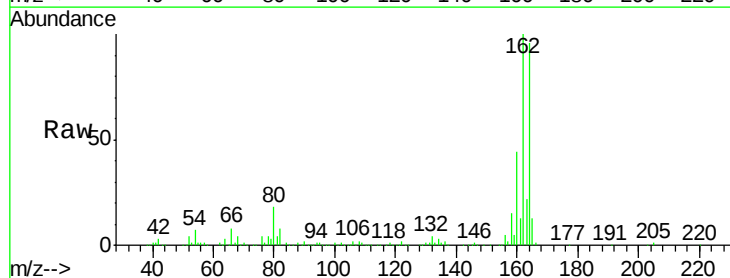


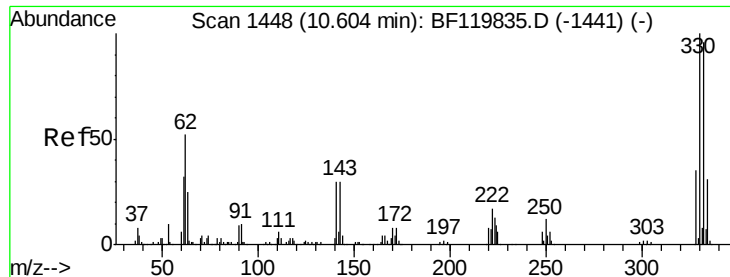




#42
 2,4,6-Tribromophenol
 Concen: 87.971 ng
 RT: 10.53 min Scan# 1435
 Delta R.T. -0.00 min
 Lab File: BF120108.D
 Acq: 21 Apr 2020 17:58

Instrument :
 BNA_F
 ClientSampleId :
 SB-1B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	76.8	115.2
141	35.1	25.1	37.7

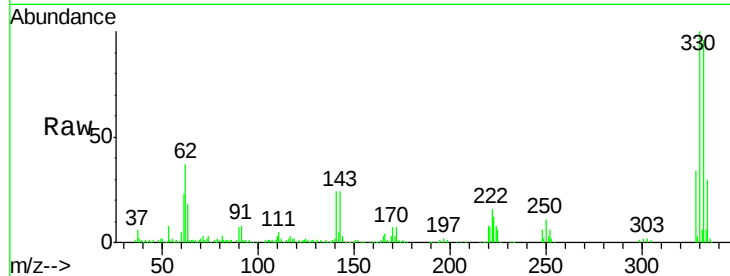


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

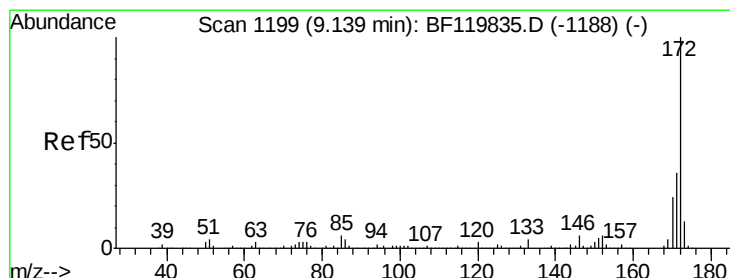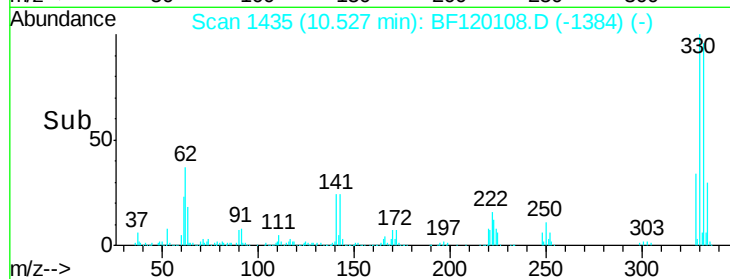
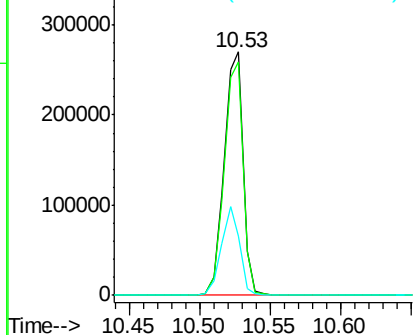



#45
 2-Fluorobiphenyl
 Concen: 78.775 ng
 RT: 9.06 min Scan# 1185
 Delta R.T. -0.01 min
 Lab File: BF120108.D
 Acq: 21 Apr 2020 17:58

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.9	43.3
170	24.2	19.4	29.2

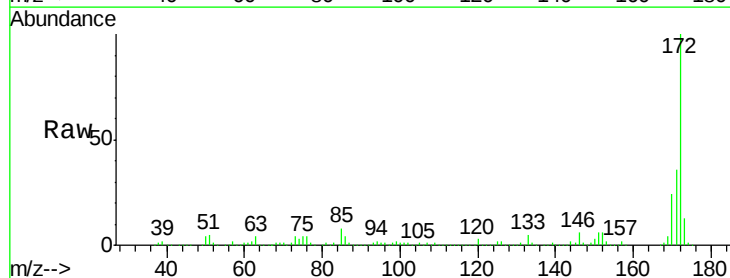

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

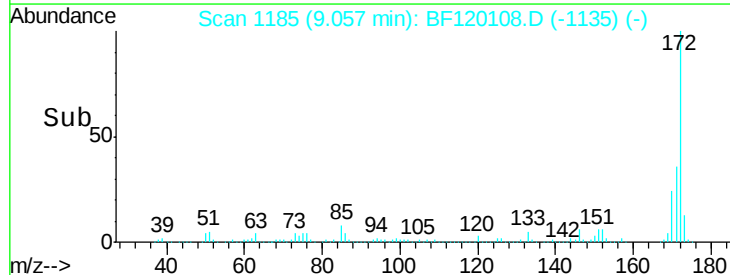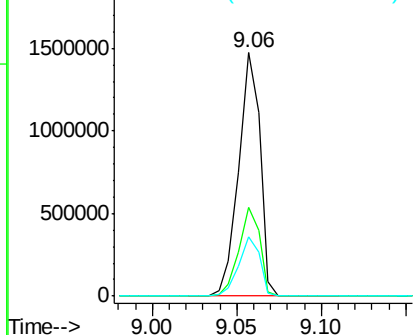

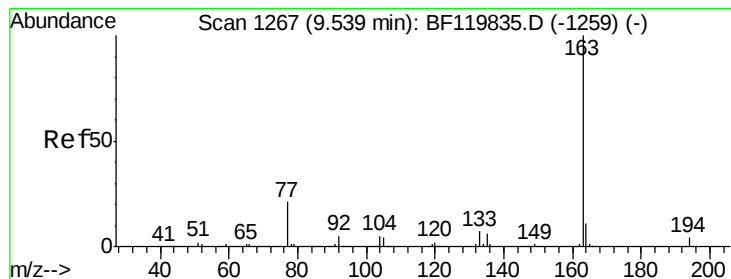

#50

Dimethylphthalate

Concen: 11.550 ng

RT: 9.45 min Scan# 1252

Delta R.T. -0.02 min

Lab File: BF120108.D

Acq: 21 Apr 2020 17:58

Instrument :

BNA_F

ClientSampleId :

SB-1B


Tot Ion:163 Resp: 208627

Ion Ratio Lower Upper

163 100

194 3.5 3.0 4.4




164 10.4 8.4 12.6

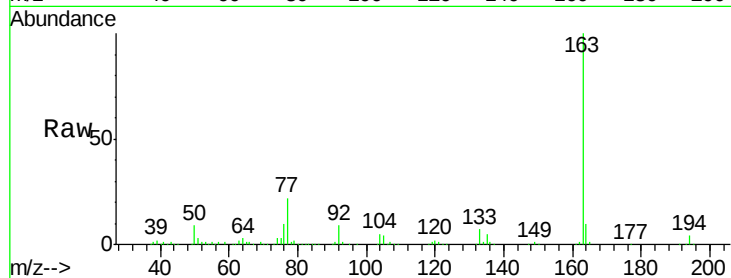

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

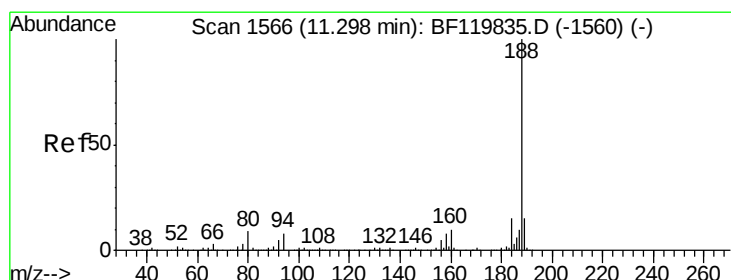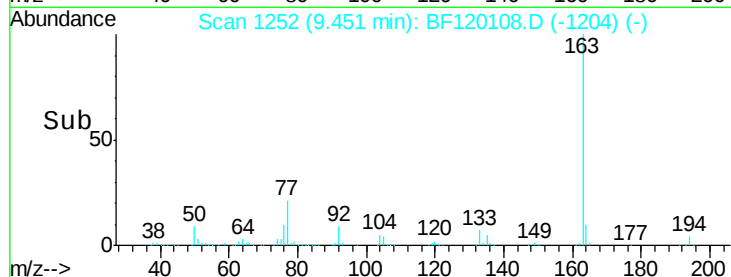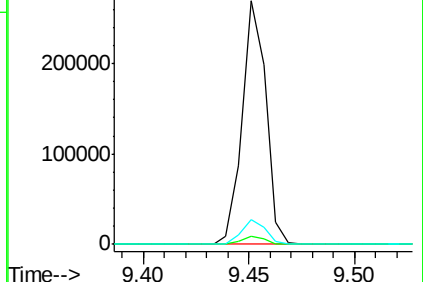

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.22 min Scan# 1552

Delta R.T. -0.01 min

Lab File: BF120108.D

Acq: 21 Apr 2020 17:58


Tgt Ion:188 Resp: 394142

Ion Ratio Lower Upper

188 100

94 9.6 6.7 10.1



80 10.5 7.4 11.2

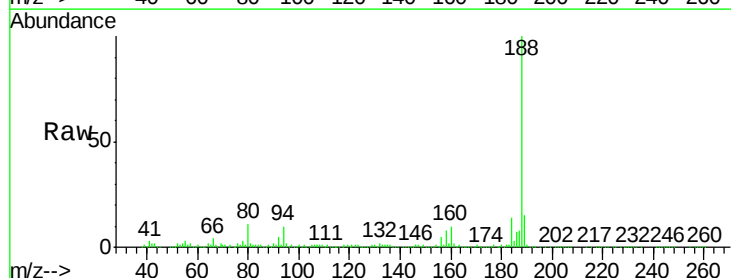


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

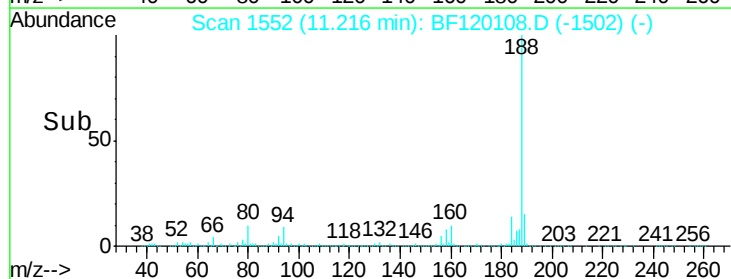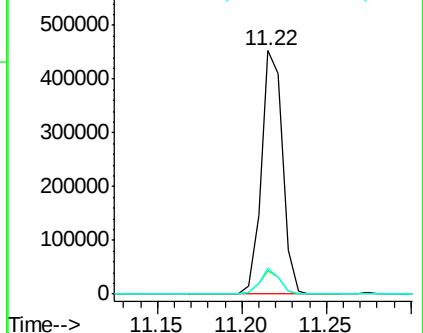

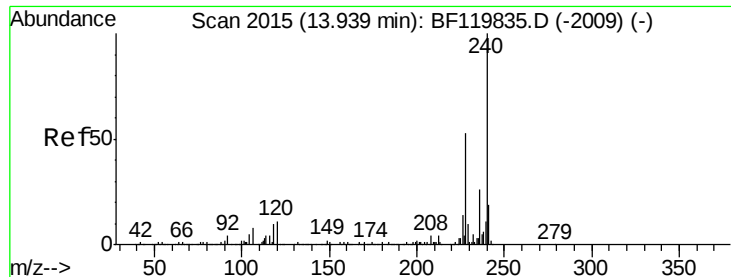

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.86 min Scan# 2002

Delta R.T. -0.01 min

Lab File: BF120108.D

Acq: 21 Apr 2020 17:58

Instrument :

BNA_F

ClientSampleId :

SB-1B


Tot Ion:240 Resp: 238160

Ion Ratio Lower Upper

240 100

120 11.6 9.0 13.6




236 27.0 20.7 31.1

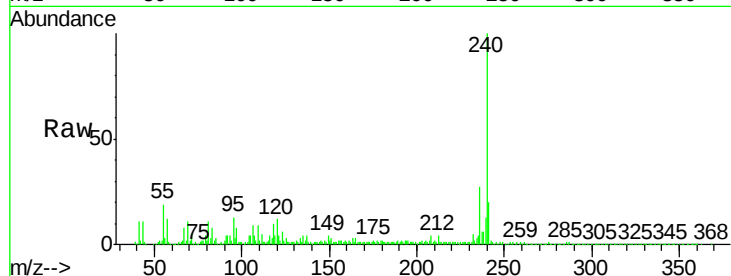

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

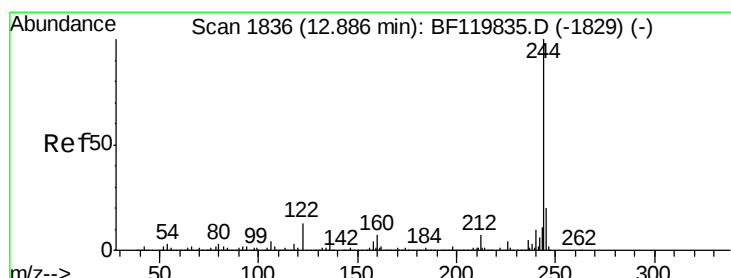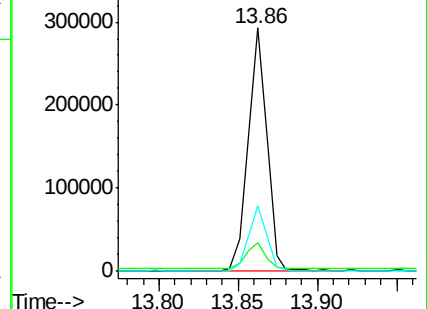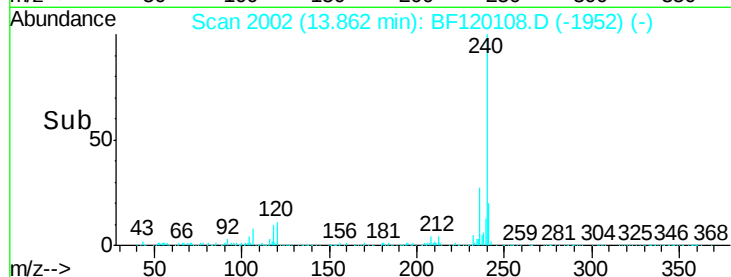

#79

Terphenyl-d14

Concen: 71.043 ng

RT: 12.81 min Scan# 1823

Delta R.T. -0.01 min

Lab File: BF120108.D

Acq: 21 Apr 2020 17:58


Tgt Ion:244 Resp: 1005527

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0



122 12.9 10.3 15.5

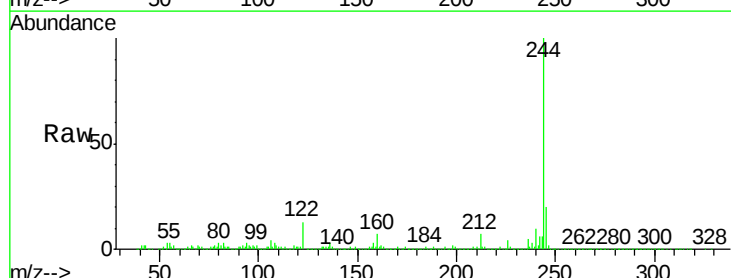


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

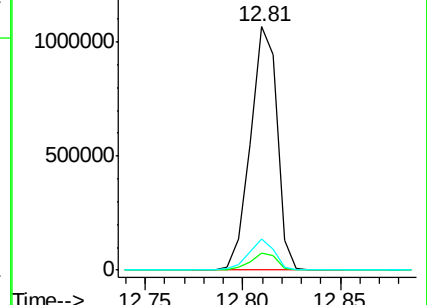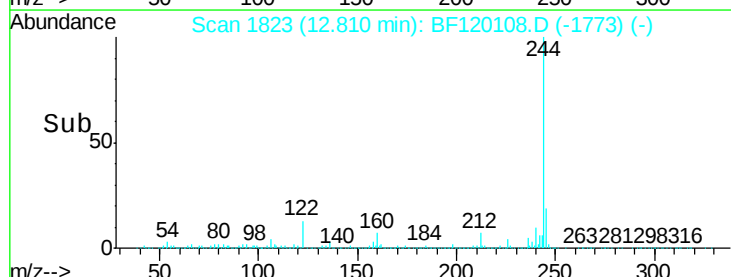


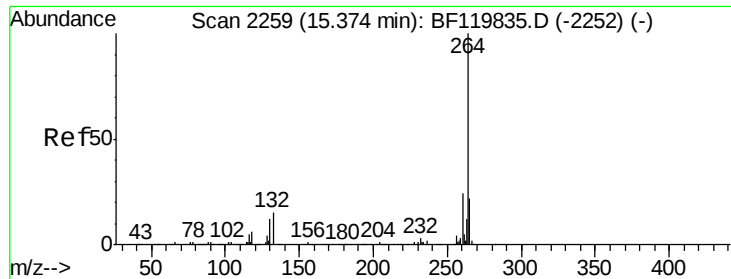

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.29 min Scan# 2244
Delta R.T. 0.01 min
Lab File: BF120108.D
Acq: 21 Apr 2020 17:58

Instrument :
BNA_F
ClientSampleId :
SB-1B

Tot Ion:	264	Resp:	252778
Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.3	28.9
265	21.2	17.6	26.4

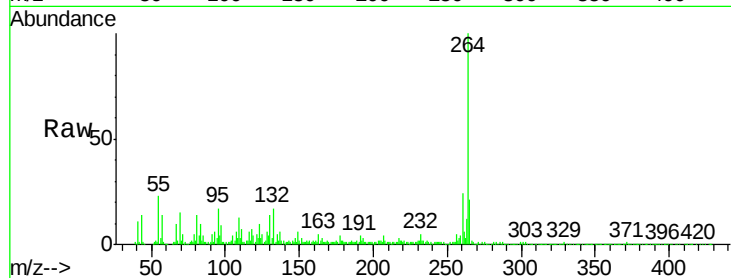

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

