


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042120\
 Data File : BF120096.D
 Acq On : 21 Apr 2020 12:06
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 21 13:48:22 2020

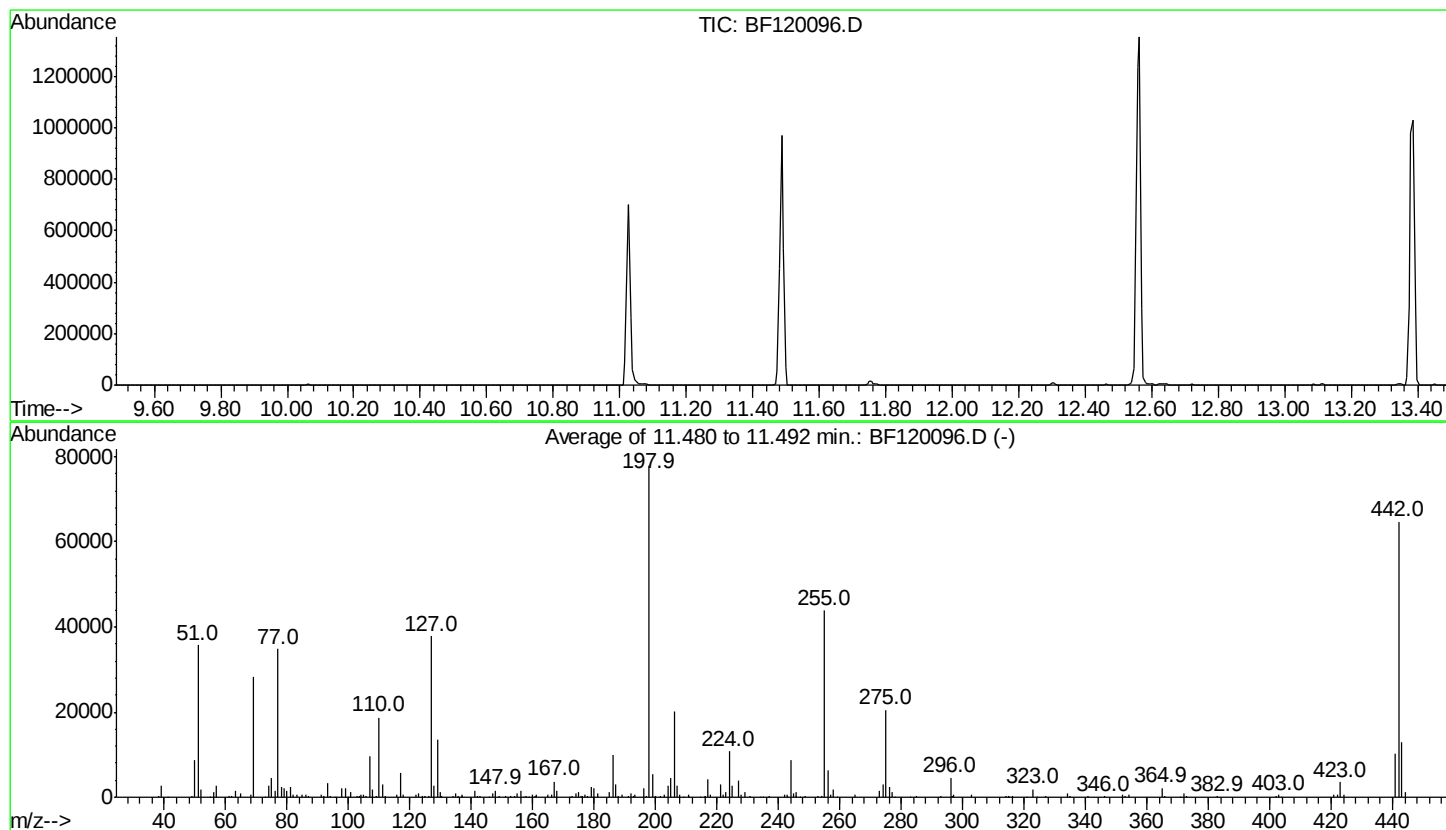

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	35717	PASS
68	69	0.00	2	1.9	534	PASS
69	198	0.00	100	36.4	28318	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	37856	PASS
197	198	0.00	2	0.2	163	PASS
198	198	100	100	100.0	77882	PASS
199	198	5	9	7.1	5521	PASS
275	198	10	60	26.3	20463	PASS
365	198	1	100	2.8	2163	PASS
441	198	0.01	100	13.1	10218	PASS
442	198	50	100	83.1	64733	PASS
443	442	15	24	19.8	12848	PASS