
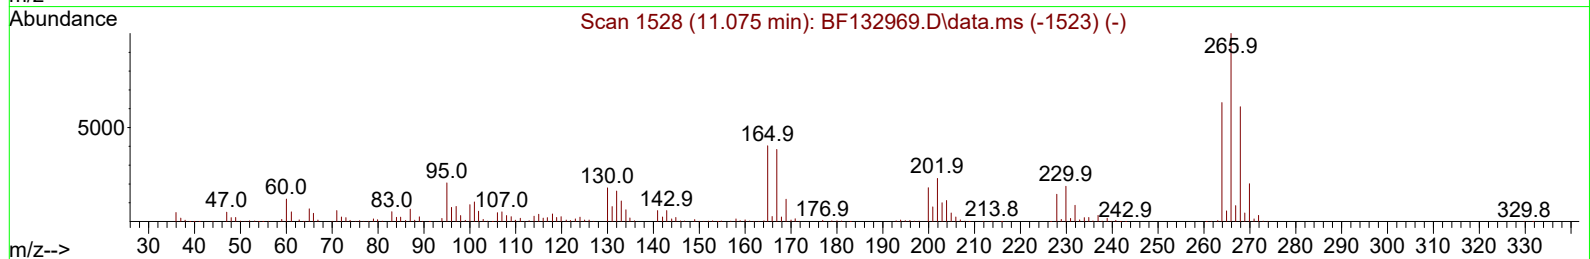
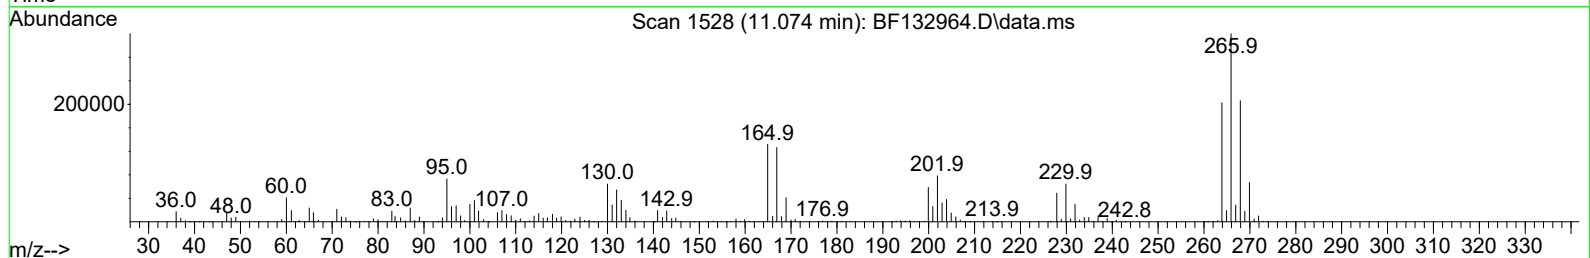


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042123\
Data File : BF132964.D
Acq On : 21 Apr 2023 12:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 06:39:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

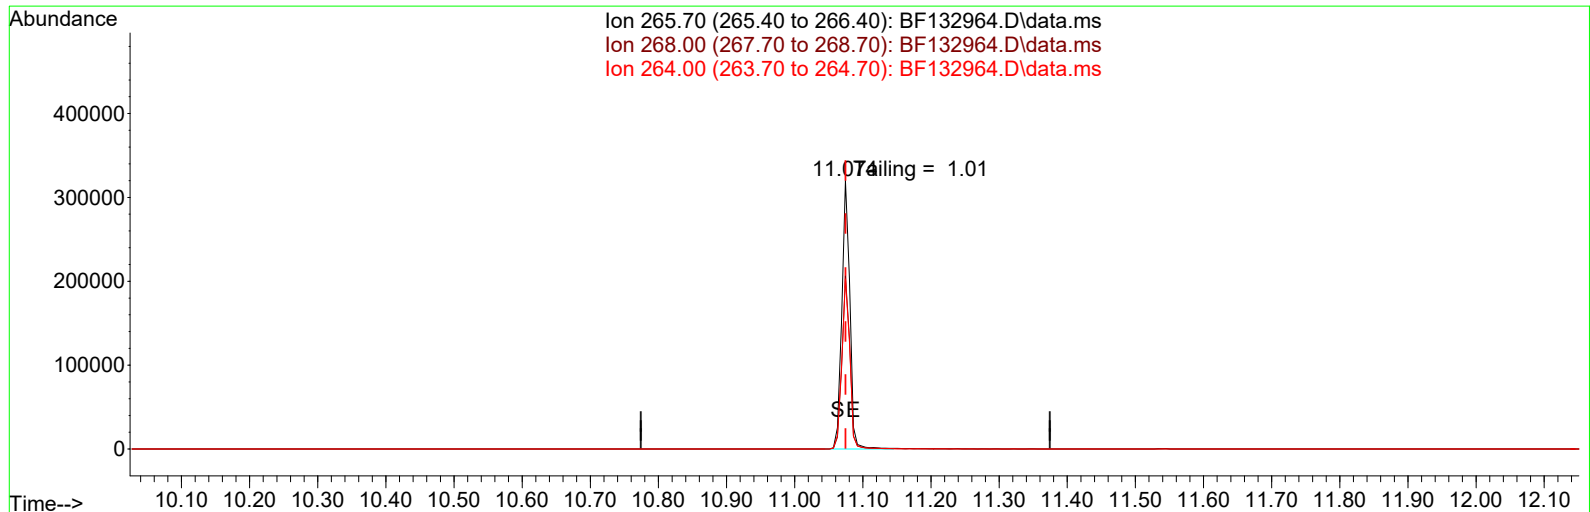

TIC: BF132964.D\data.ms

(70) Pentachlorophenol (C)




11.074min (-0.000) 461711.32 ng

response 263115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.46
264.00	63.30	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042123\
Data File : BF132964.D
Acq On : 21 Apr 2023 12:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 06:39:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

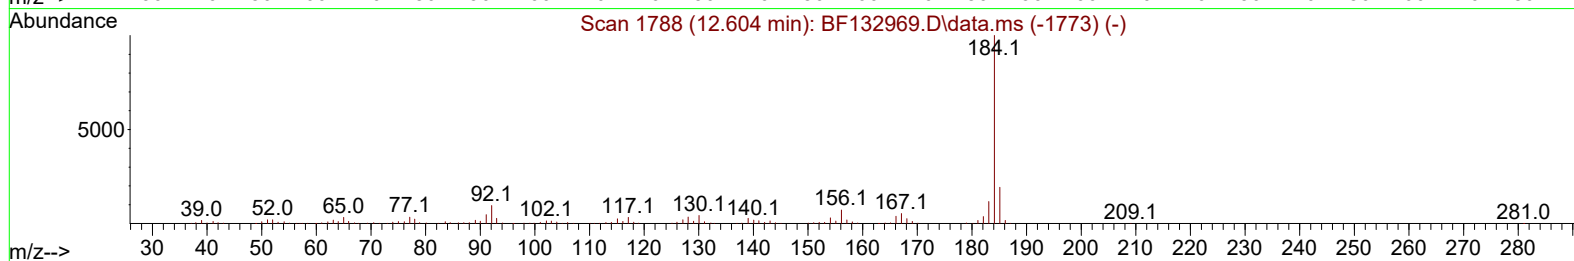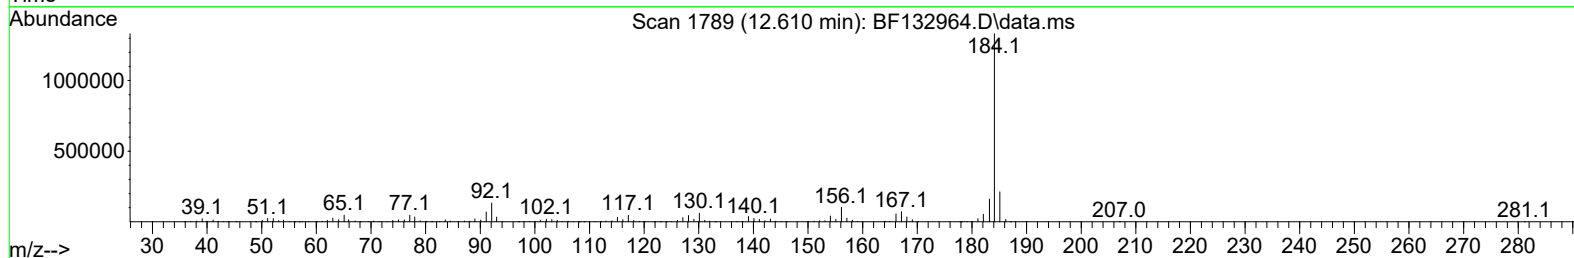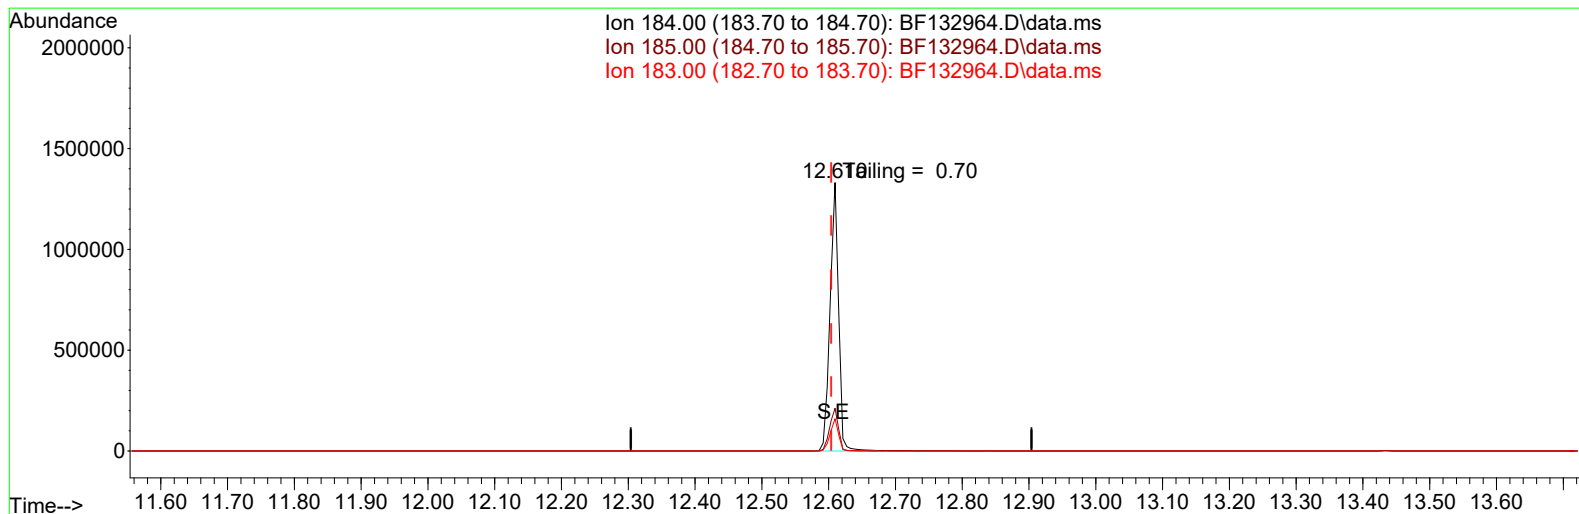

TIC: BF132964.D\data.ms

(77) Benzidine

12.610min (+ 0.006) 9254.01 ng m

response 1186196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	15.94
183.00	11.70	12.06
0.00	0.00	0.00