
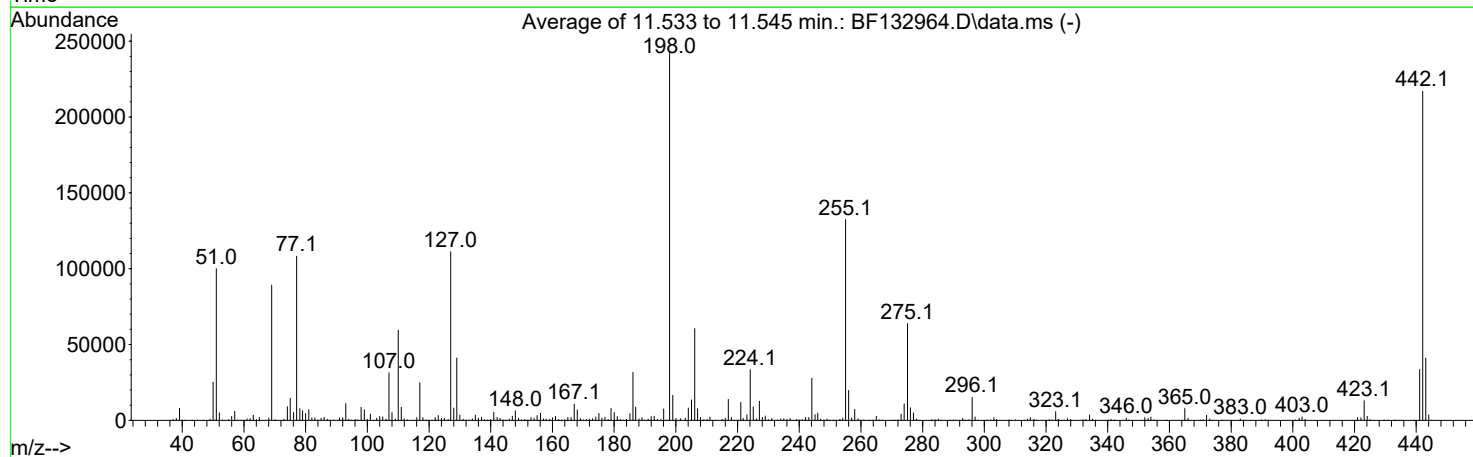


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042123\
 Data File : BF132964.D
 Acq On : 21 Apr 2023 12:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 22 03:30:56 2023

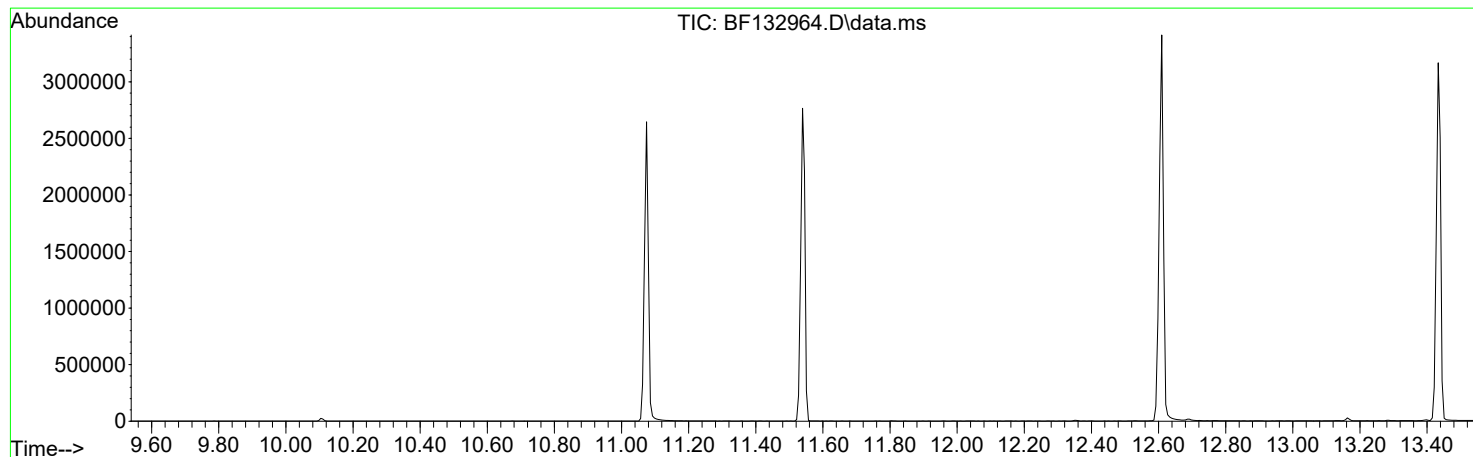

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	100053	PASS
68	69	0.00	2	1.7	1534	PASS
69	198	0.00	100	36.7	89125	PASS
70	69	0.00	2	0.5	461	PASS
127	198	10	80	45.8	111149	PASS
197	198	0.00	2	0.1	359	PASS
198	198	100	100	100.0	242539	PASS
199	198	5	9	6.8	16604	PASS
275	198	10	60	26.3	63829	PASS
365	198	1	100	3.2	7821	PASS
441	198	0.01	100	13.8	33521	PASS
442	442	50	100	100.0	216909	PASS
443	442	15	24	18.9	41086	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/21/2023	BNA_F	<u>BF132964.D</u>
Compound Name	Response	Retention Time
DDT	533293	13.433
DDD	4099	13.163
DDE		12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4099	537392	0.76

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042123\
Data File : BF132964.D
Acq On : 21 Apr 2023 12:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 22 06:39:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

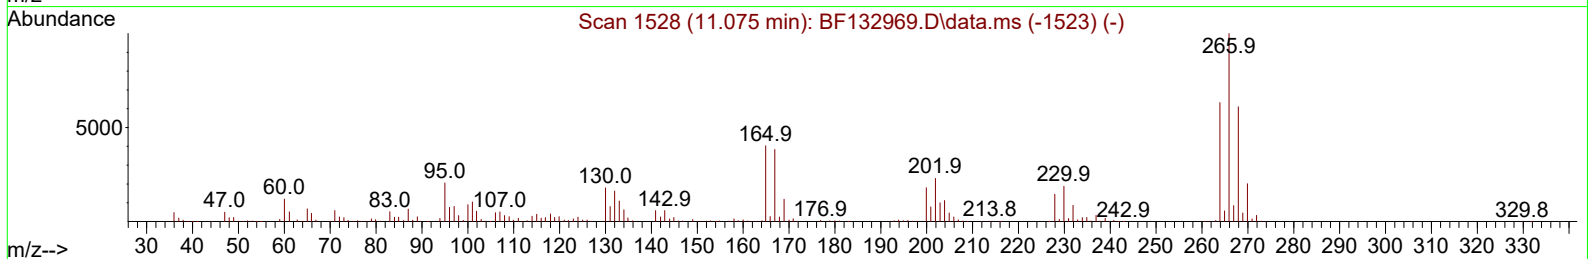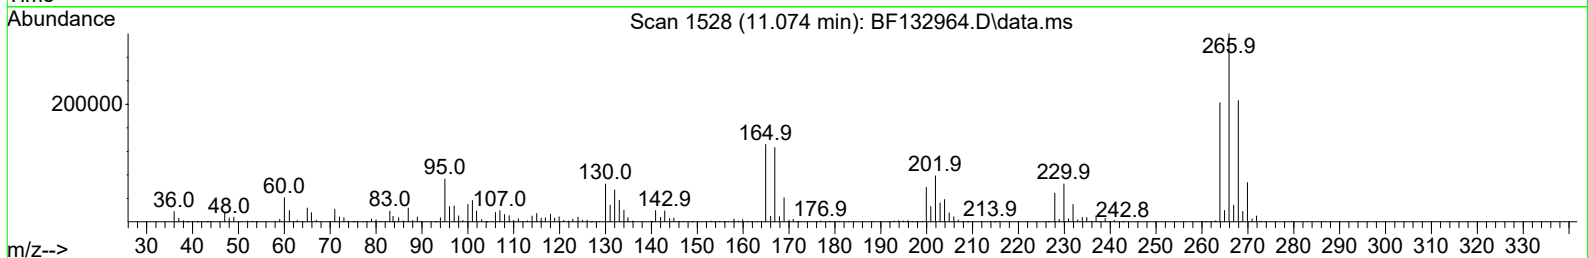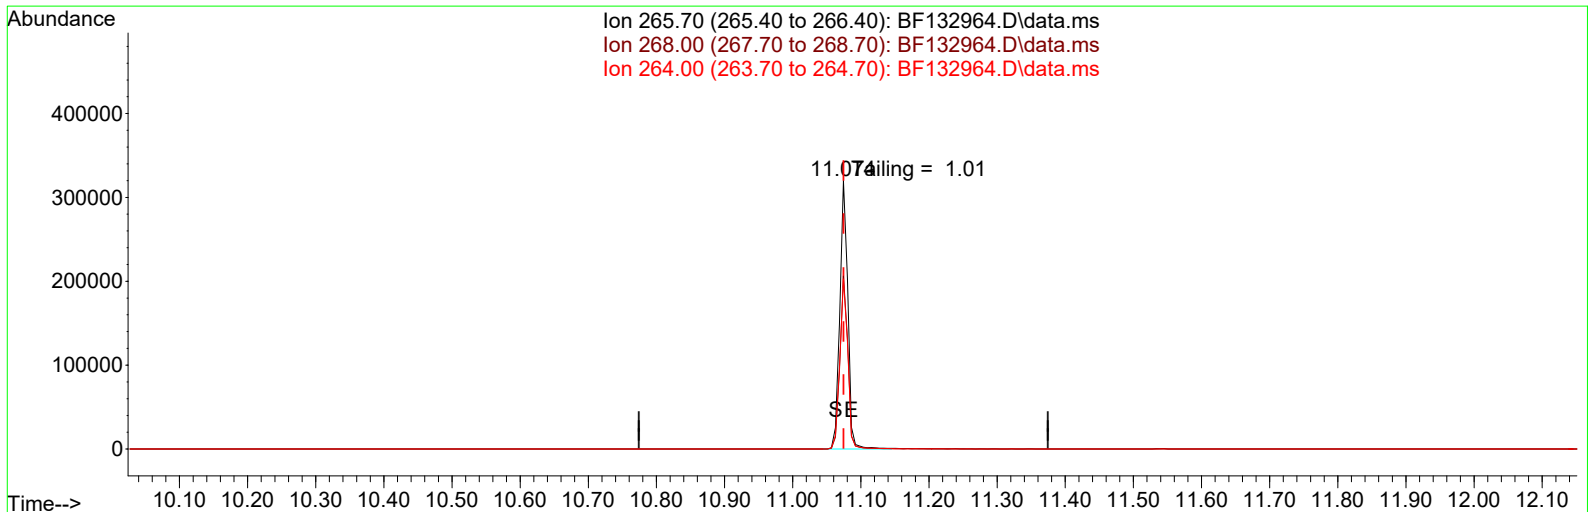

TIC: BF132964.D\data.ms

(70) Pentachlorophenol (C)

11.074min (-0.000) 461711.32 ng




response 263115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.46
264.00	63.30	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042123\
Data File : BF132964.D
Acq On : 21 Apr 2023 12:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 22 06:39:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 22 03:30:56 2023
Response via : Initial Calibration

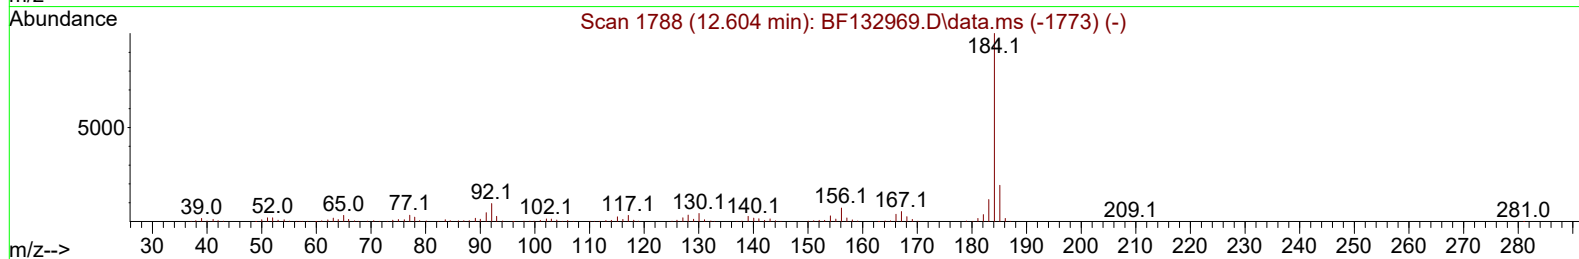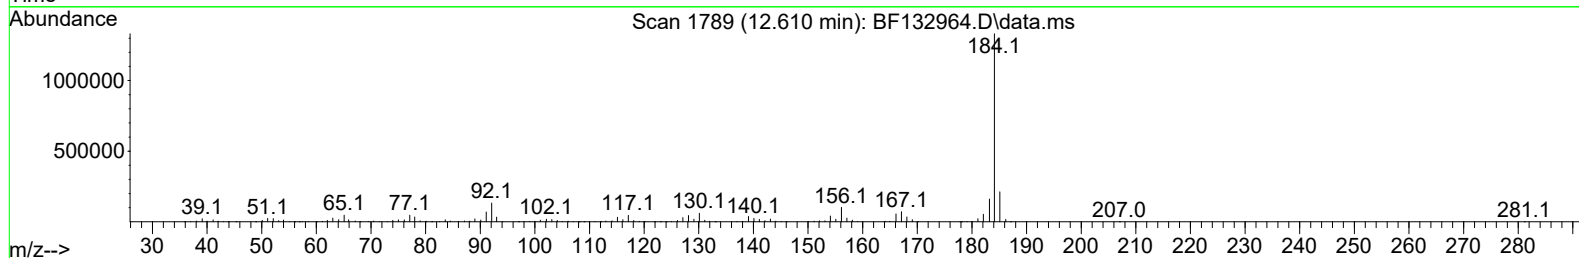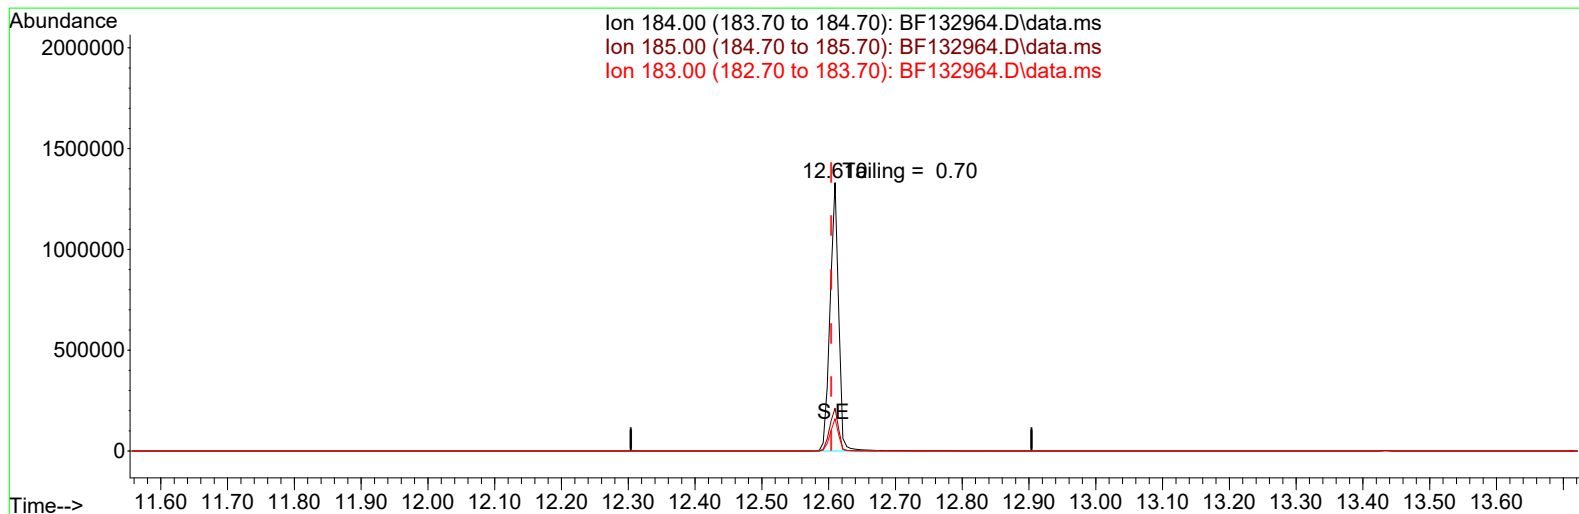

TIC: BF132964.D\data.ms

(77) Benzidine

12.610min (+ 0.006) 9254.01 ng m

response 1186196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	15.94
183.00	11.70	12.06
0.00	0.00	0.00