
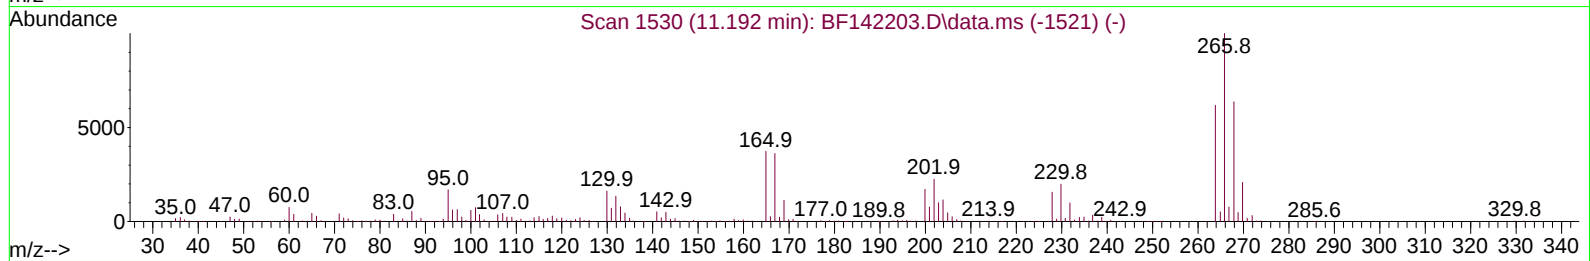
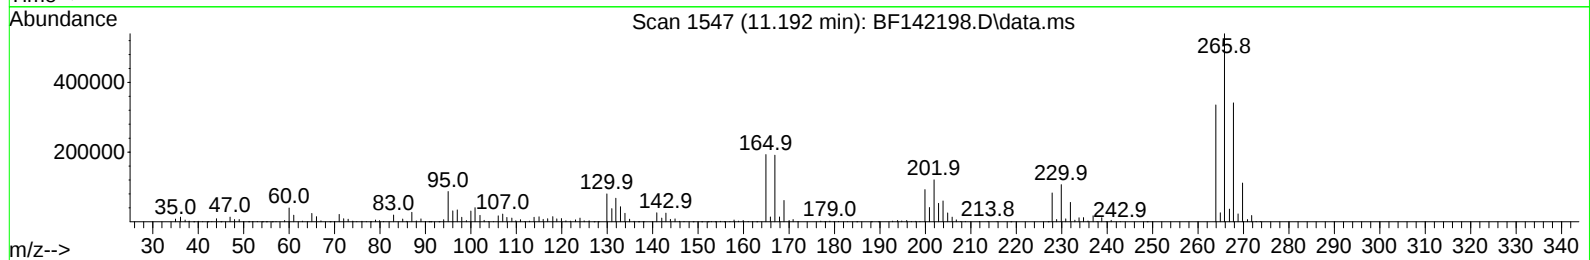


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042125\
Data File : BF142198.D
Acq On : 21 Apr 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 02:45:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 22 02:14:30 2025
Response via : Initial Calibration

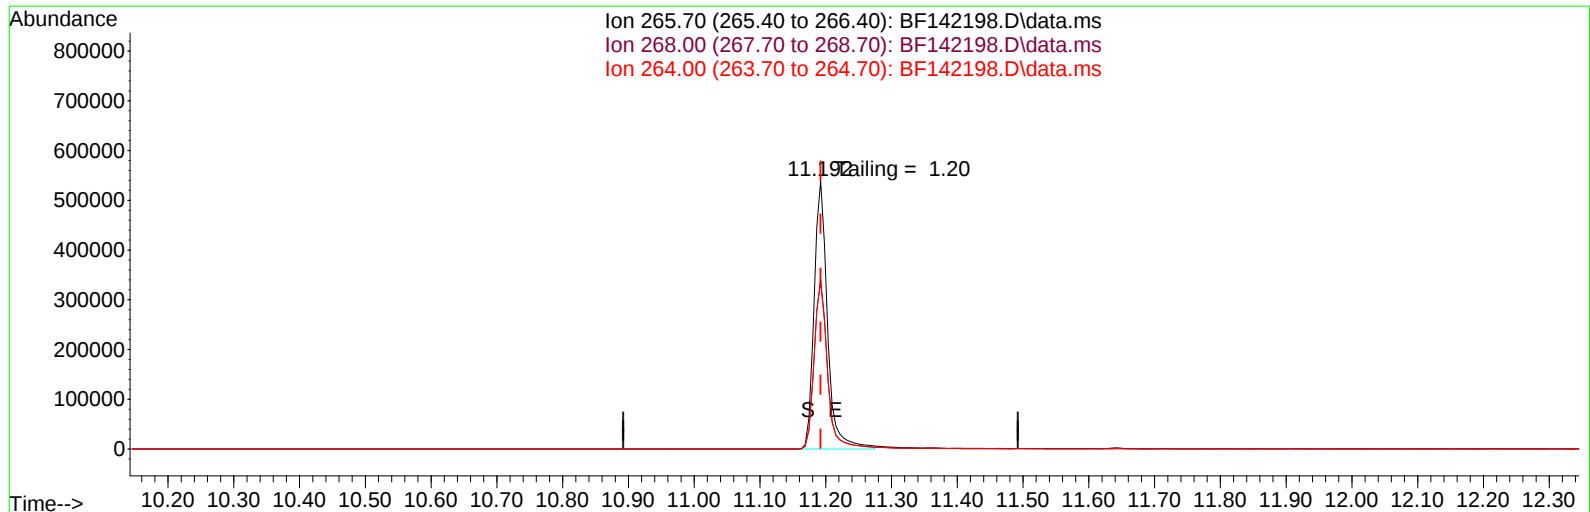

TIC: BF142198.D\data.ms

(70) Pentachlorophenol (C)




11.192min (-0.000) 204849.53 ng

response 780132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.26
264.00	61.80	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042125\
Data File : BF142198.D
Acq On : 21 Apr 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 02:45:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 22 02:14:30 2025
Response via : Initial Calibration

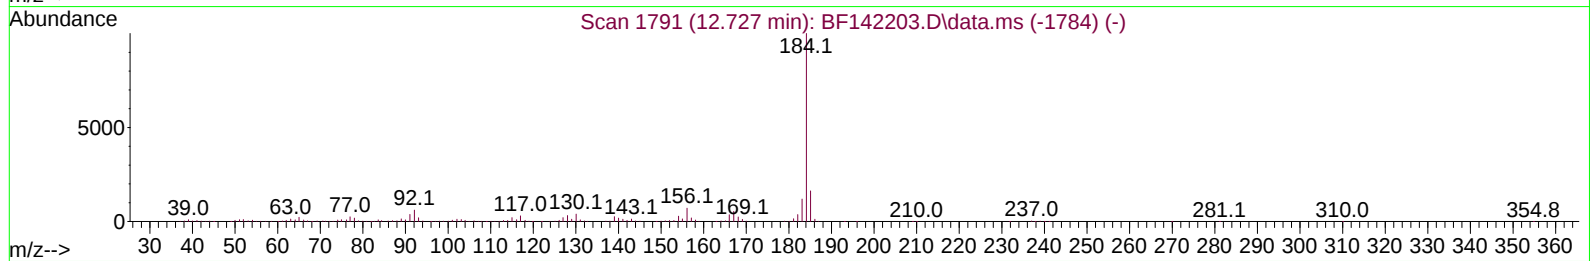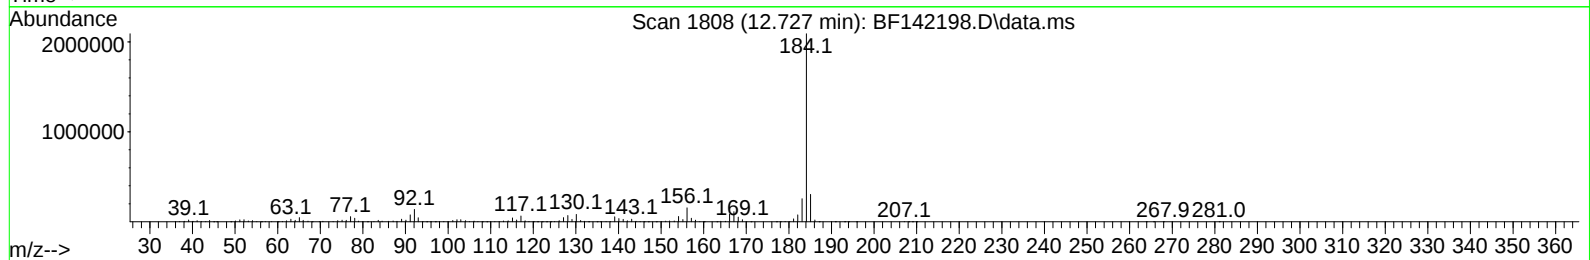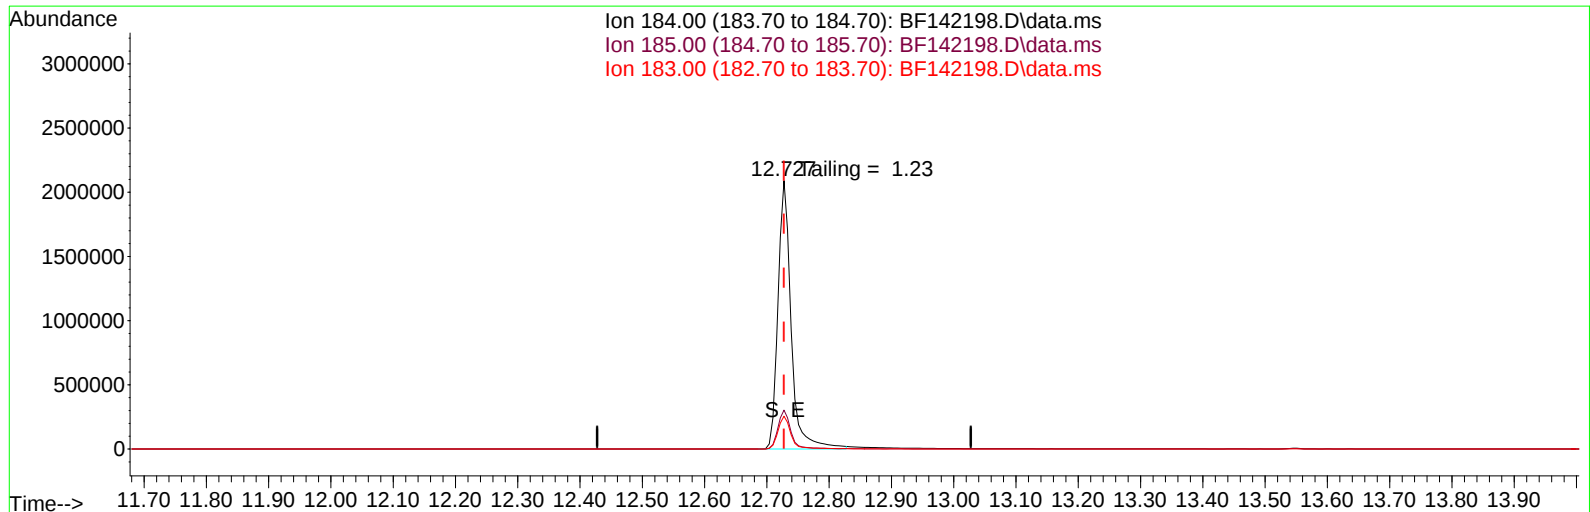

TIC: BF142198.D\data.ms

(77) Benzidine

12.727min (-0.000) 321157.70 ng

response 3162201

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.30	14.52
183.00	12.00	12.25
0.00	0.00	0.00