
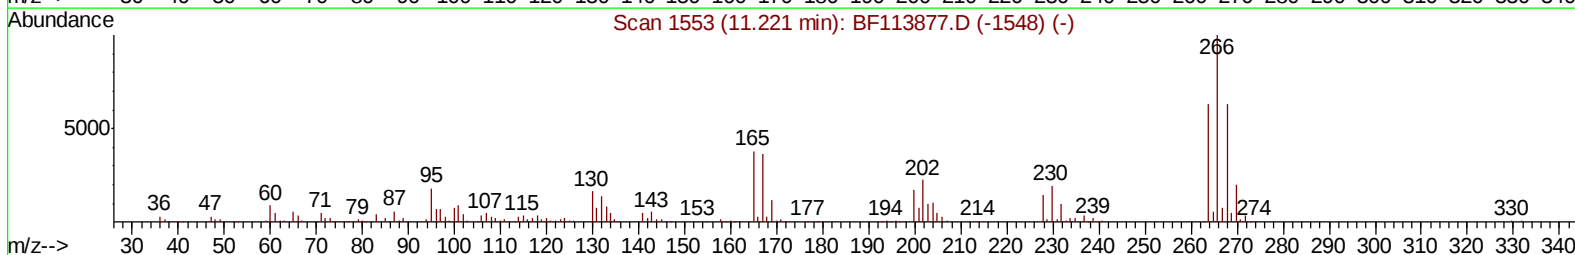
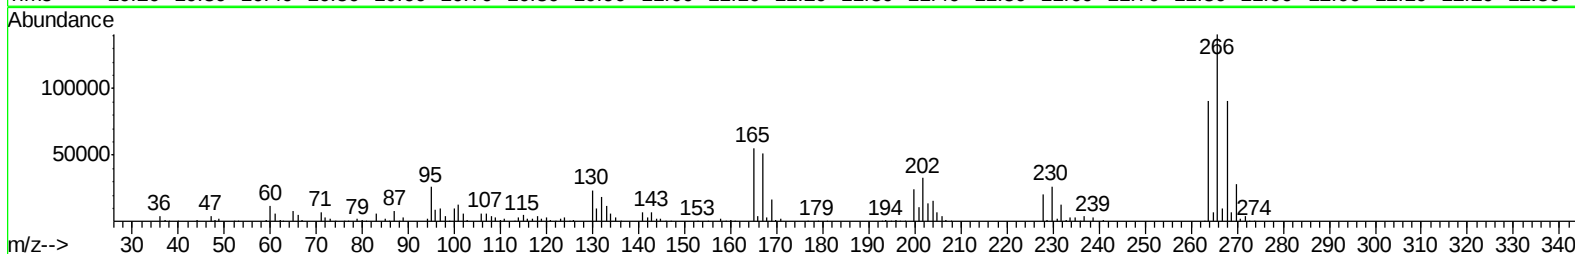


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042219\
Data File : BF113883.D
Acq On : 22 Apr 2019 17:47
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 05:09:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 03:32:35 2019
Response via : Initial Calibration

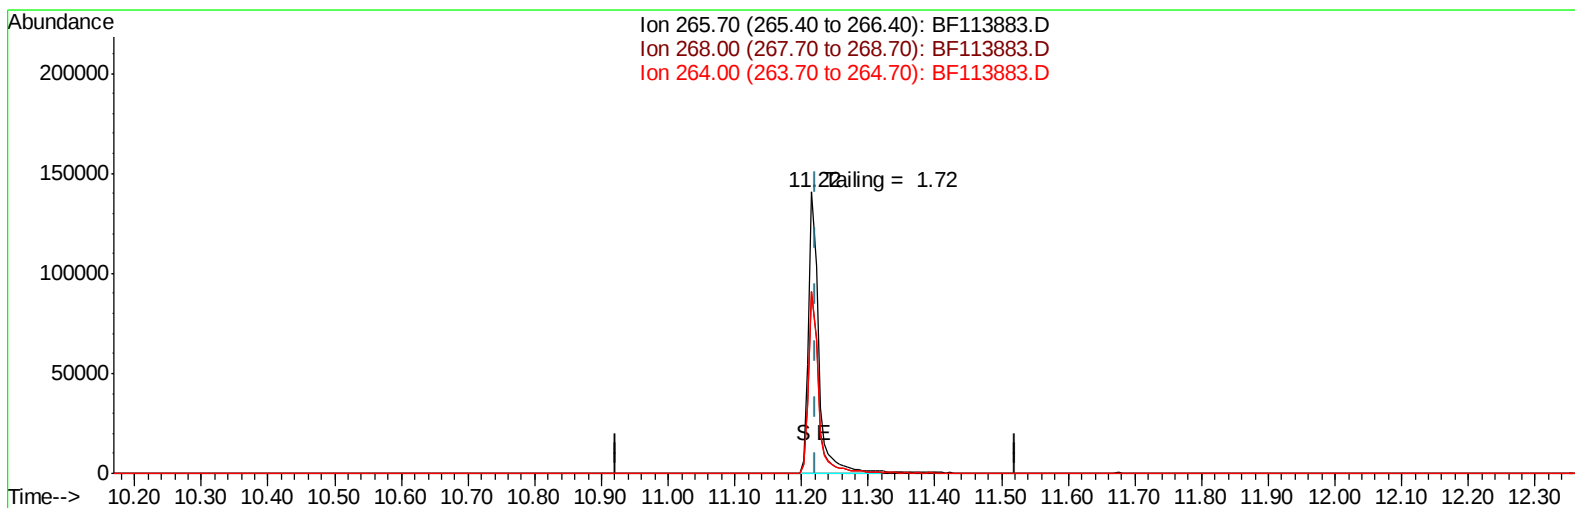

TIC: BF113883.D

(70) Pentachlorophenol (C)




11.216min (-0.006) 40994.12ng

response 142968

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	64.47
264.00	63.80	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042219\
 Data File : BF113883.D
 Acq On : 22 Apr 2019 17:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 05:09:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 03:32:35 2019
 Response via : Initial Calibration

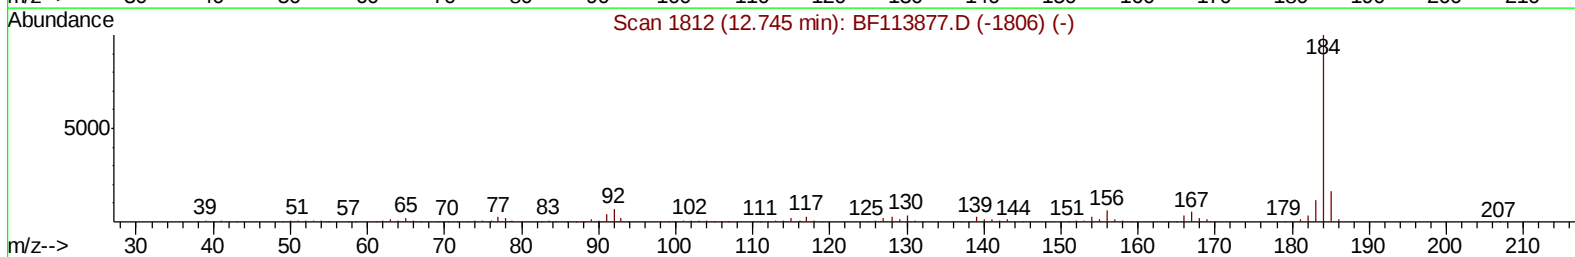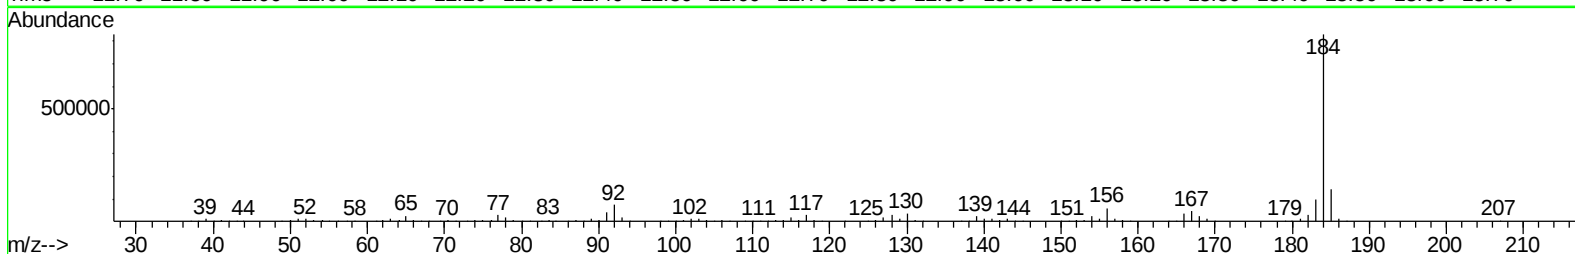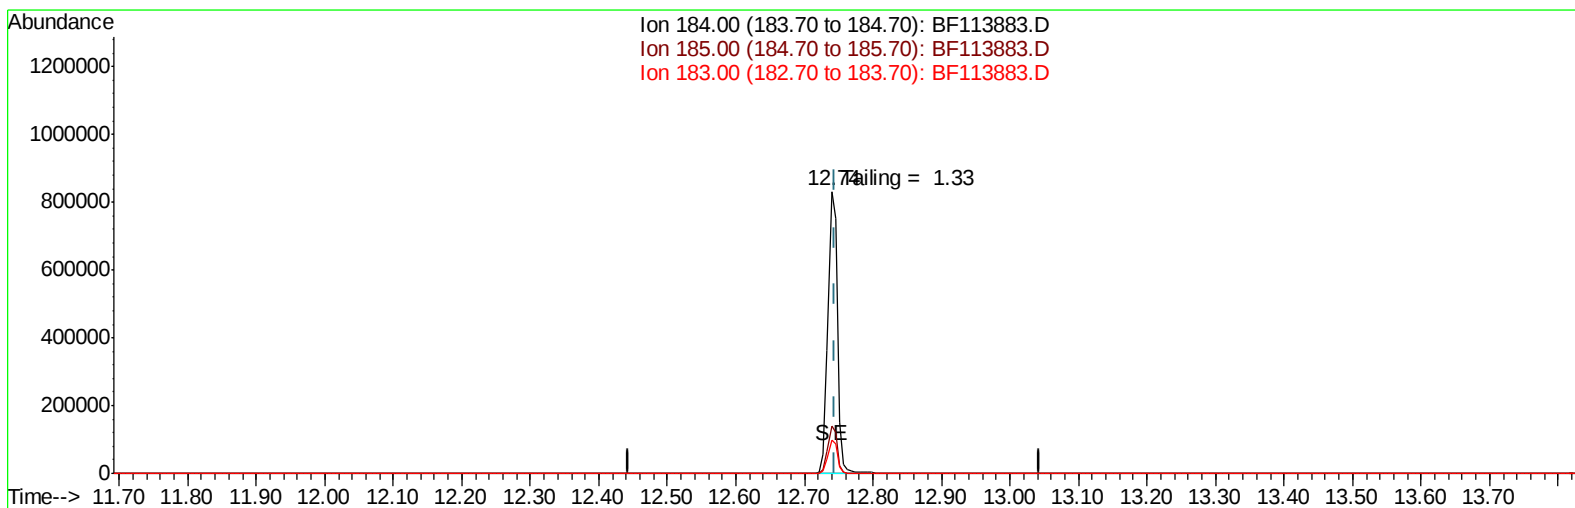

TIC: BF113883.D

(77) Benzidine

12.739min (-0.005) 0.00ng

response 785733

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.88
183.00	11.70	11.74
0.00	0.00	0.00