


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042219\
 Data File : BF113908.D
 Acq On : 23 Apr 2019 5:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

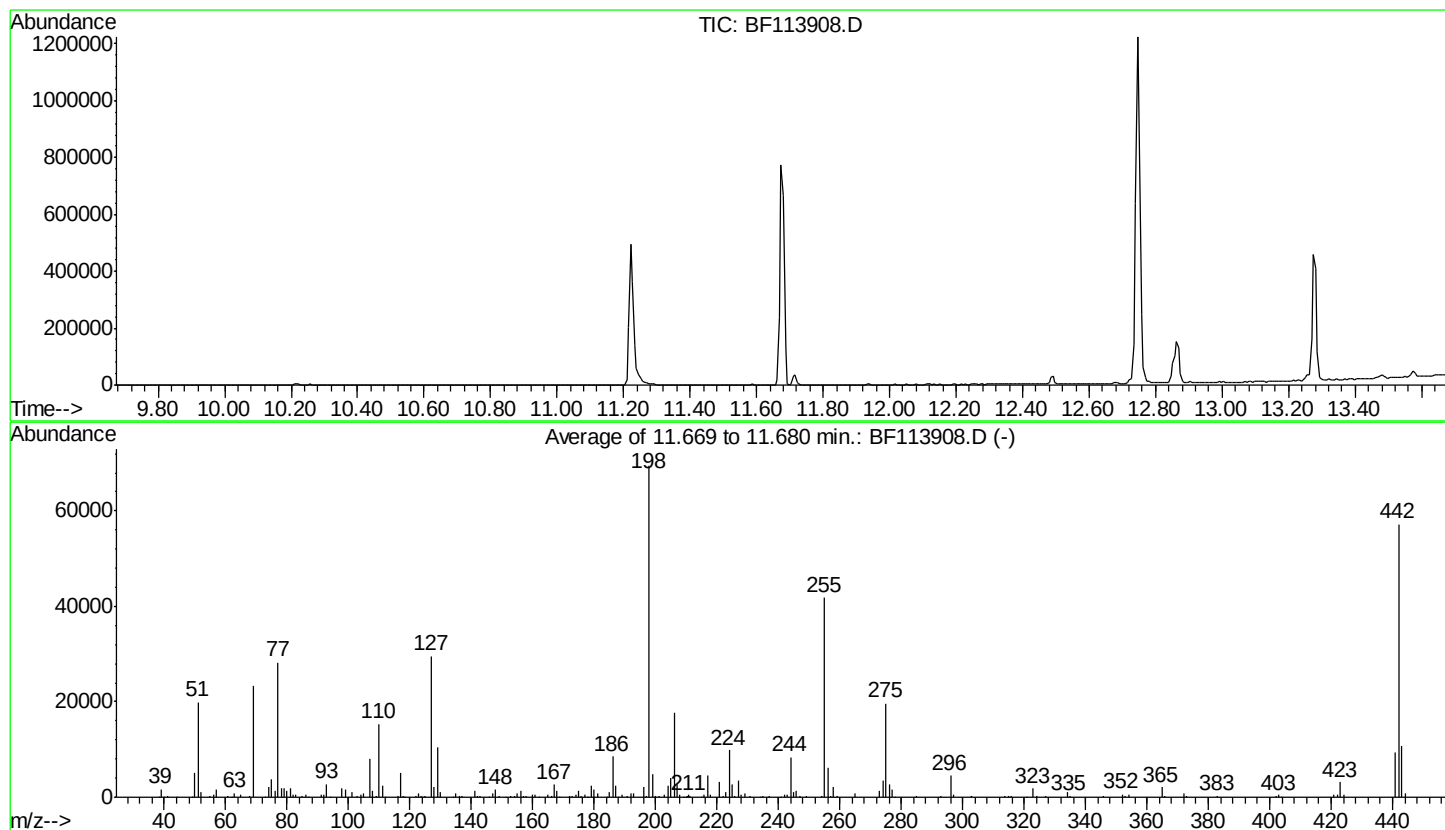

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	19862	PASS
68	69	0.00	2	1.2	283	PASS
69	198	0.00	100	33.5	23272	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	29632	PASS
197	198	0.00	2	0.6	391	PASS
198	198	100	100	100.0	69490	PASS
199	198	5	9	6.9	4797	PASS
275	198	10	60	28.3	19679	PASS
365	198	1	100	3.1	2129	PASS
441	198	0.01	100	13.6	9437	PASS
442	198	50	100	82.4	57261	PASS
443	442	15	24	18.7	10712	PASS