

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
 Data File : BF120124.D
 Acq On : 22 Apr 2020 12:06
 Operator : MA/SJ
 Sample : PB128358BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128358BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.281	538	543	546	rBV	4376082	4436521	78.54%	12.252%
2	6.322	714	720	723	rBV	3979134	4308769	76.28%	11.899%
3	6.675	777	780	784	rBV	937118	752764	13.33%	2.079%
4	6.833	802	807	810	rBV	3948936	3543200	62.73%	9.785%
5	7.245	871	877	880	rBV	2830236	2971894	52.61%	8.207%
6	7.963	995	999	1002	rBV	1299721	1015643	17.98%	2.805%
7	9.045	1177	1183	1186	rBV	5846727	5383517	95.31%	14.867%
8	9.716	1293	1297	1300	rBV	1457848	1183309	20.95%	3.268%
9	10.510	1427	1432	1435	rBV	3721085	3479434	61.60%	9.609%
10	11.204	1546	1550	1553	rBV	1388287	1257110	22.25%	3.472%
11	12.798	1815	1821	1824	rBV	5668212	5648715	100.00%	15.599%
12	13.839	1994	1998	2002	rBV	1265474	1165441	20.63%	3.218%
13	15.251	2233	2238	2242	rBV	911016	1065657	18.87%	2.943%


Sum of corrected areas: 36211974

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120124.D
Acq On : 22 Apr 2020 12:06
Operator : MA/SJ
Sample : PB128358BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128358BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

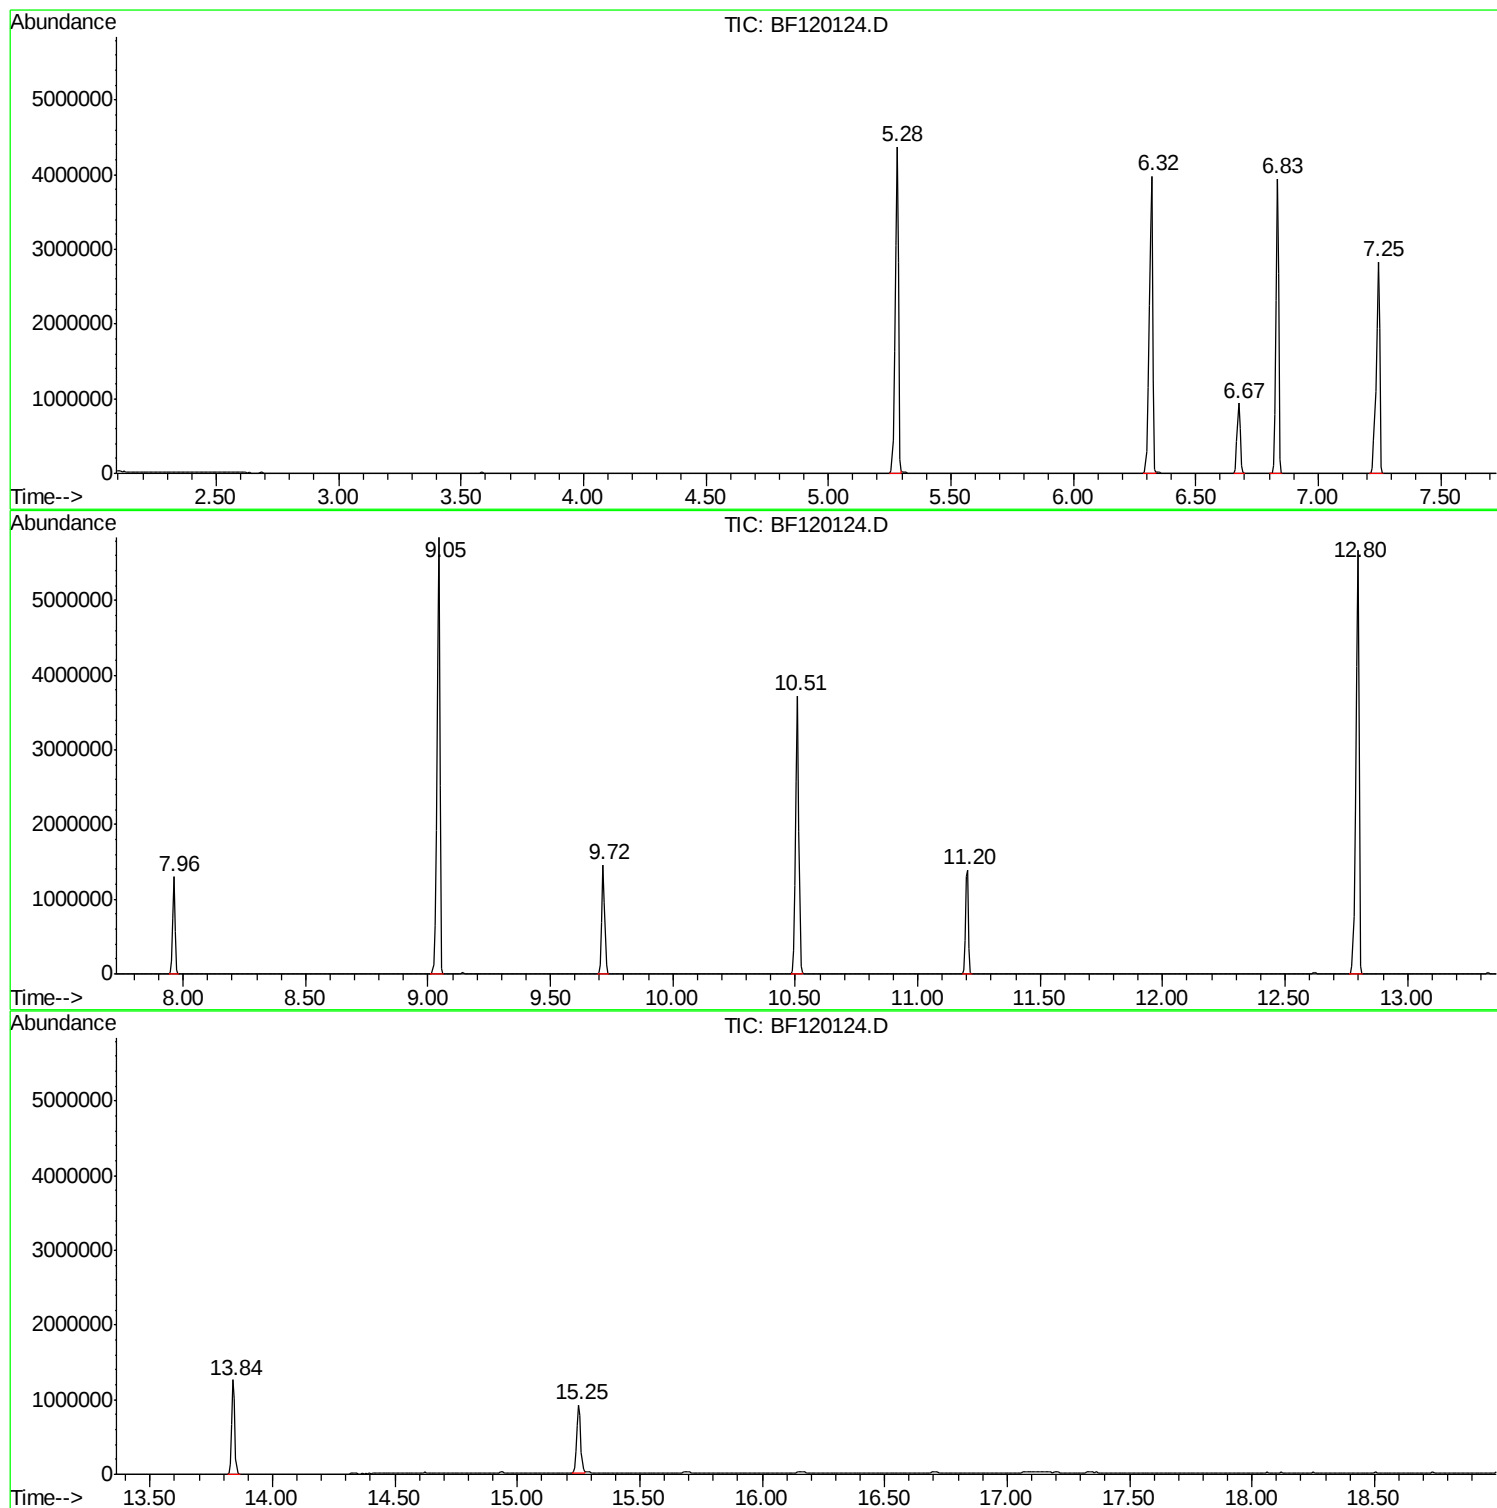

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120124.D
Acq On : 22 Apr 2020 12:06
Operator : MA/SJ
Sample : PB128358BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128358BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120124.D
Acq On : 22 Apr 2020 12:06
Operator : MA/SJ
Sample : PB128358BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128358BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc