

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
 Data File : BF120127.D
 Acq On : 22 Apr 2020 13:26
 Operator : MA/SJ
 Sample : L2327-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-4-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.469	61	65	75	rVB	463622	615931	11.11%	1.708%
2	3.328	205	211	218	rVB2	36079	66106	1.19%	0.183%
3	4.204	354	360	366	rVB	87723	112032	2.02%	0.311%
4	4.410	391	395	401	rBV	168771	187251	3.38%	0.519%
5	4.881	471	475	487	rVB	202491	224936	4.06%	0.624%
6	5.287	539	544	547	rBV	4053476	3937849	71.04%	10.919%
7	6.322	714	720	723	rBV	3247697	3432798	61.93%	9.518%
8	6.675	777	780	784	rBV	936055	748924	13.51%	2.077%
9	6.834	802	807	810	rBV	4040247	3663116	66.08%	10.157%
10	7.245	871	877	880	rBV	2842943	3031992	54.70%	8.407%
11	7.963	994	999	1001	rBV	1181675	984548	17.76%	2.730%
12	9.045	1177	1183	1186	rBV	6021476	5316548	95.91%	14.741%
13	9.716	1293	1297	1300	rBV	1380380	1099620	19.84%	3.049%
14	10.510	1426	1432	1435	rBV	3646689	3367906	60.76%	9.338%
15	11.198	1545	1549	1553	rBV	1339762	1157792	20.89%	3.210%
16	11.739	1638	1641	1644	rBV	113122	106587	1.92%	0.296%
17	12.539	1771	1777	1787	rBV	506073	473301	8.54%	1.312%
18	12.798	1815	1821	1824	rBV	5489873	5543055	100.00%	15.369%
19	13.839	1994	1998	2002	rBV	1332468	1068509	19.28%	2.963%
20	15.251	2233	2238	2242	rBV	836088	926558	16.72%	2.569%


Sum of corrected areas: 36065359

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120127.D
Acq On : 22 Apr 2020 13:26
Operator : MA/SJ
Sample : L2327-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

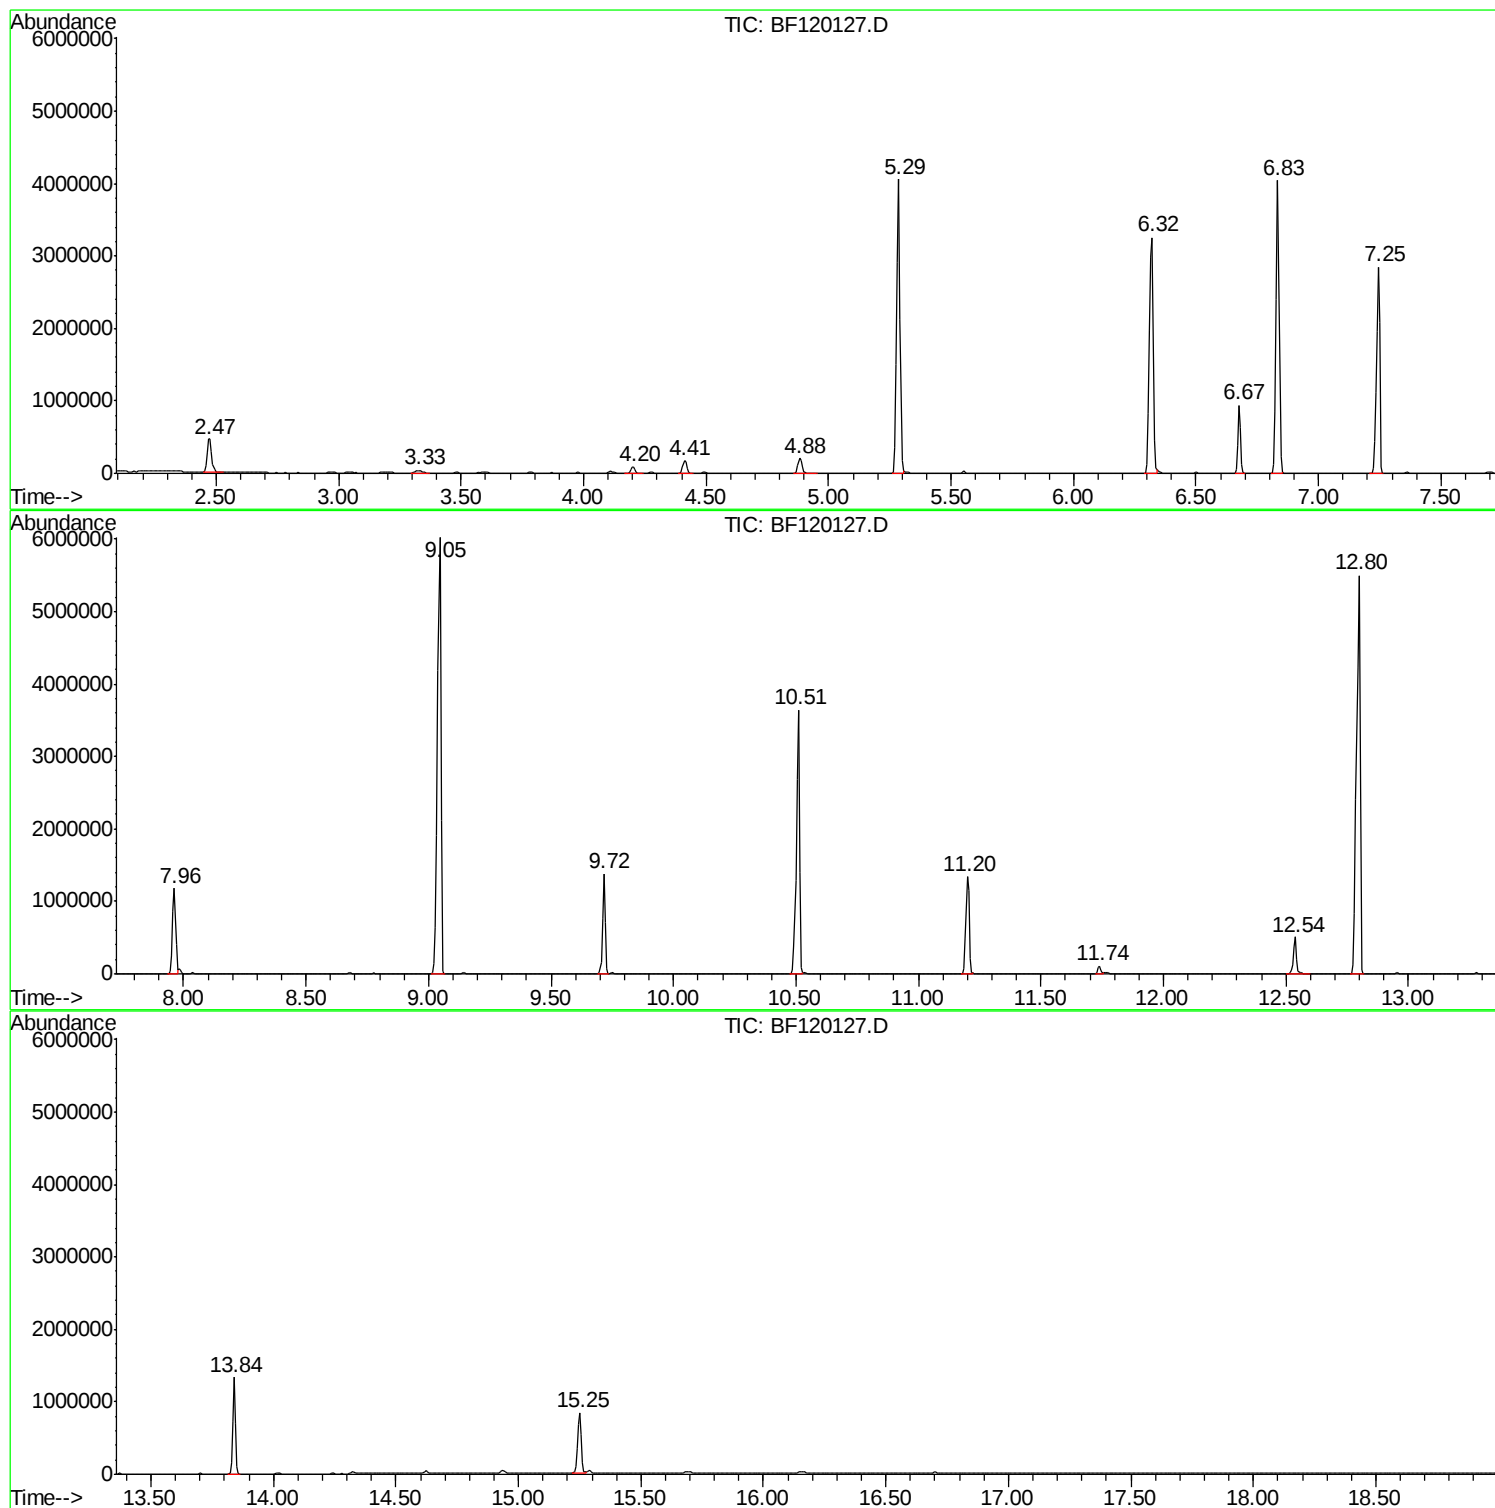

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120127.D
Acq On : 22 Apr 2020 13:26
Operator : MA/SJ
Sample : L2327-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120127.D
Acq On : 22 Apr 2020 13:26
Operator : MA/SJ
Sample : L2327-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
