

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
 Data File : BF120128.D
 Acq On : 22 Apr 2020 13:53
 Operator : MA/SJ
 Sample : L2327-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-4-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.469	60	65	77	rVB	427031	543242	9.15%	1.429%
2	4.199	355	359	367	rVB	77496	98355	1.66%	0.259%
3	4.410	391	395	402	rVB	144681	168493	2.84%	0.443%
4	4.881	471	475	486	rVB	176416	194194	3.27%	0.511%
5	5.287	539	544	547	rBV	4315287	4296522	72.39%	11.299%
6	6.322	714	720	723	rBV	3607216	3788030	63.82%	9.962%
7	6.675	776	780	784	rBV	1007527	818227	13.79%	2.152%
8	6.834	802	807	810	rBV	4254354	3891695	65.57%	10.234%
9	7.245	871	877	880	rBV	2953898	3230931	54.44%	8.497%
10	7.963	995	999	1002	rBV	1315658	1053388	17.75%	2.770%
11	9.045	1177	1183	1186	rBV	6237080	5707831	96.17%	15.011%
12	9.716	1292	1297	1300	rBV	1487445	1191870	20.08%	3.134%
13	10.510	1426	1432	1435	rBV	3878012	3611653	60.85%	9.498%
14	11.198	1546	1549	1553	rBV	1469477	1241657	20.92%	3.265%
15	12.798	1815	1821	1824	rBV	5921962	5935232	100.00%	15.609%
16	13.274	1899	1902	1906	rBV	142460	122917	2.07%	0.323%
17	13.839	1994	1998	2002	rBV	1280348	1127618	19.00%	2.965%
18	15.251	2233	2238	2242	rBV	884941	1003611	16.91%	2.639%


Sum of corrected areas: 38025466

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120128.D
Acq On : 22 Apr 2020 13:53
Operator : MA/SJ
Sample : L2327-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

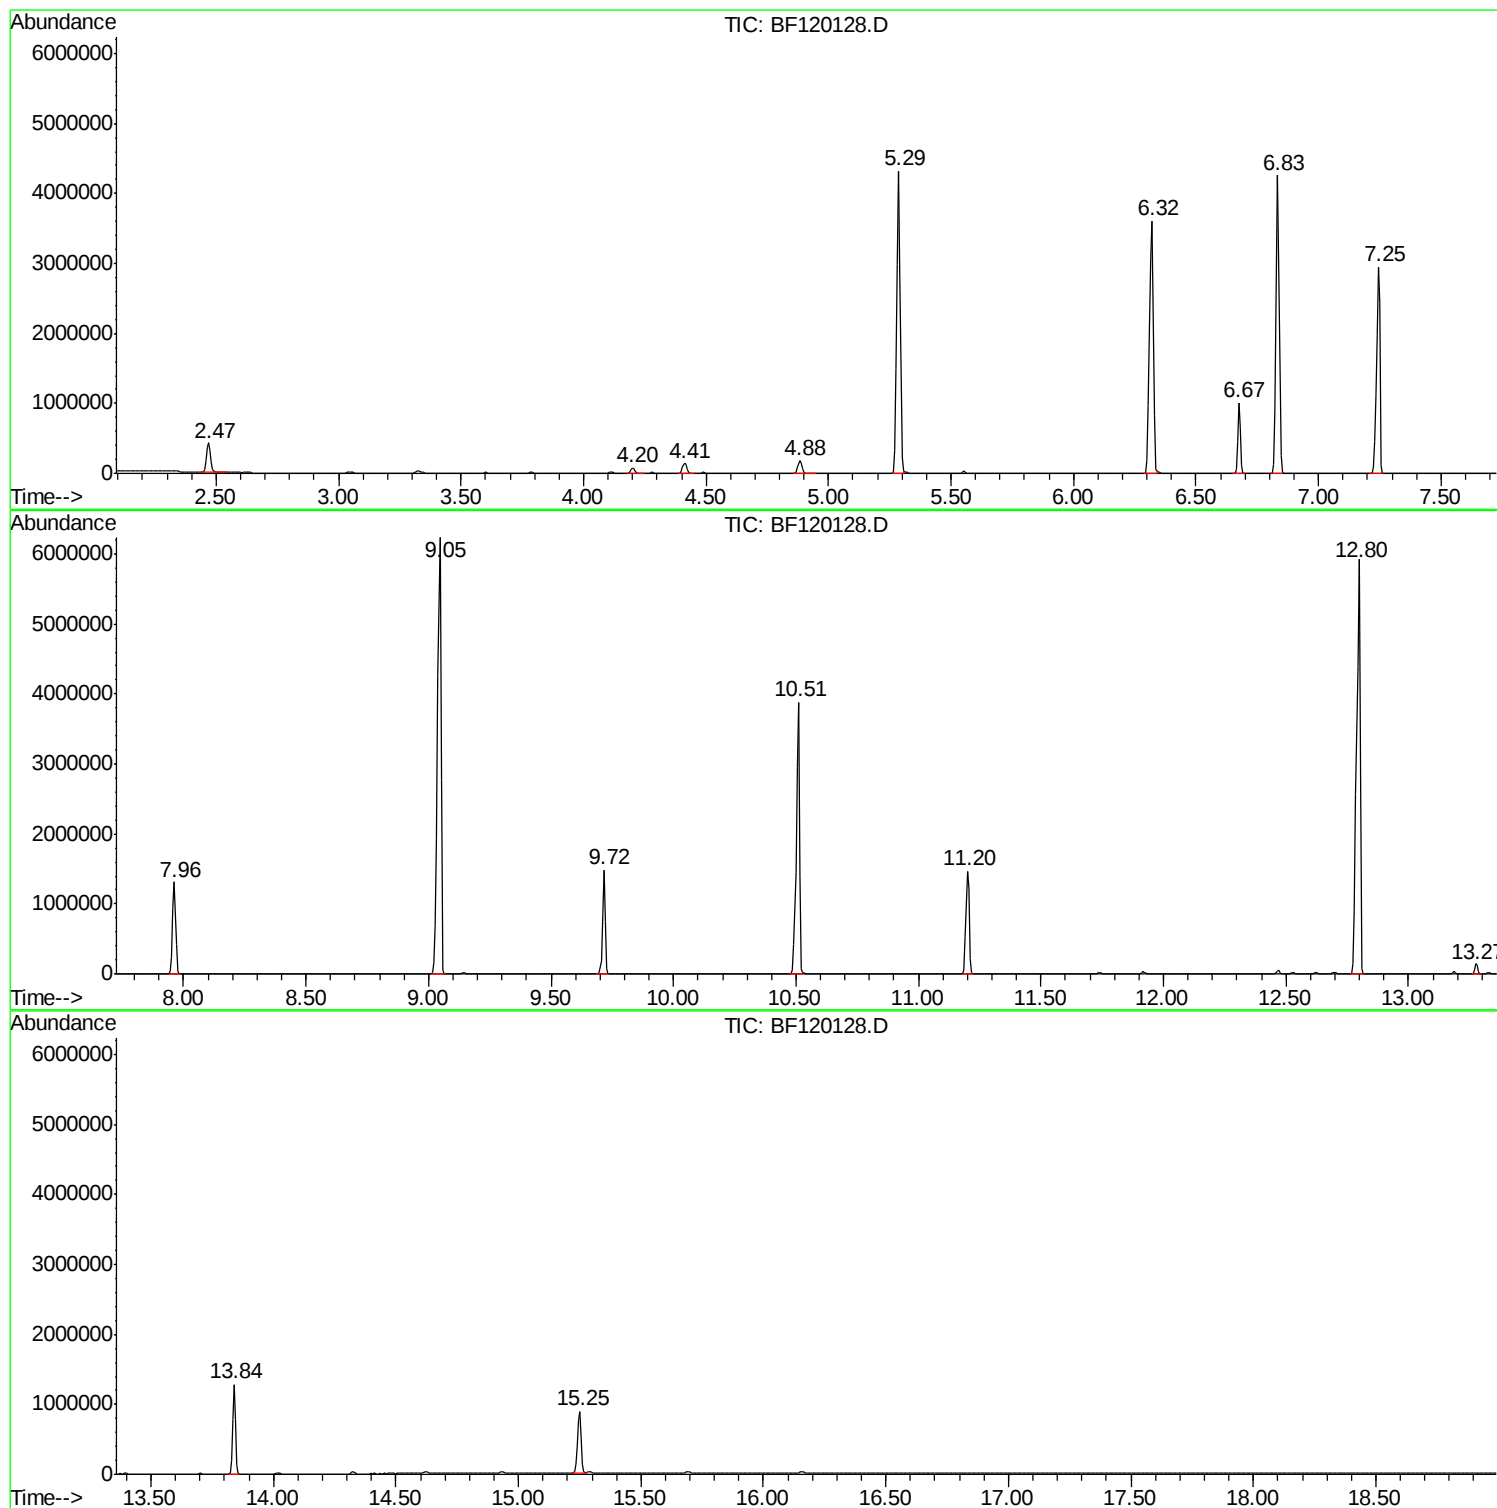

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120128.D
Acq On : 22 Apr 2020 13:53
Operator : MA/SJ
Sample : L2327-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120128.D
Acq On : 22 Apr 2020 13:53
Operator : MA/SJ
Sample : L2327-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc