

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
 Data File : BF120129.D
 Acq On : 22 Apr 2020 14:20
 Operator : MA/SJ
 Sample : L2327-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-4-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.469	60	65	72	rVB	461287	606576	10.76%	1.645%
2	3.322	205	210	218	rVB	33926	64777	1.15%	0.176%
3	4.199	352	359	364	rBV	96232	116823	2.07%	0.317%
4	4.410	391	395	401	rVB	177498	190973	3.39%	0.518%
5	4.881	471	475	483	rVB	216949	232443	4.12%	0.630%
6	5.287	539	544	547	rBV	3986446	3876266	68.74%	10.511%
7	6.322	714	720	722	rBV	3187185	3417496	60.61%	9.267%
8	6.675	776	780	784	rBV	961302	802299	14.23%	2.176%
9	6.834	802	807	810	rBV	3957845	3597006	63.79%	9.754%
10	7.245	871	877	880	rBV	2822451	3001434	53.23%	8.139%
11	7.963	994	999	1002	rBV	1323003	1071782	19.01%	2.906%
12	9.045	1177	1183	1186	rBV	5996410	5365466	95.15%	14.550%
13	9.716	1292	1297	1300	rBV	1550270	1223418	21.70%	3.318%
14	10.510	1426	1432	1435	rBV	3763431	3447234	61.14%	9.348%
15	11.198	1546	1549	1553	rBV	1510953	1296443	22.99%	3.516%
16	11.739	1638	1641	1650	rBV2	79730	83595	1.48%	0.227%
17	12.527	1772	1775	1782	rBV2	58649	64350	1.14%	0.174%
18	12.798	1815	1821	1824	rBV	5902693	5638699	100.00%	15.291%
19	13.274	1899	1902	1906	rVB	122053	107894	1.91%	0.293%
20	13.839	1994	1998	2002	rBV	1375286	1146817	20.34%	3.110%
21	14.327	2077	2081	2084	rBV	70490	66247	1.17%	0.180%
22	14.621	2127	2131	2136	rBV	109676	99736	1.77%	0.270%
23	14.933	2181	2184	2189	rVB	101151	109228	1.94%	0.296%
24	15.251	2233	2238	2242	rBV	914632	1001185	17.76%	2.715%
25	15.292	2242	2245	2250	rVB	85885	102121	1.81%	0.277%
26	15.692	2308	2313	2319	rBV	59243	86569	1.54%	0.235%
27	16.157	2387	2392	2398	rBV	35163	60079	1.07%	0.163%


Sum of corrected areas: 36876956

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120129.D
Acq On : 22 Apr 2020 14:20
Operator : MA/SJ
Sample : L2327-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

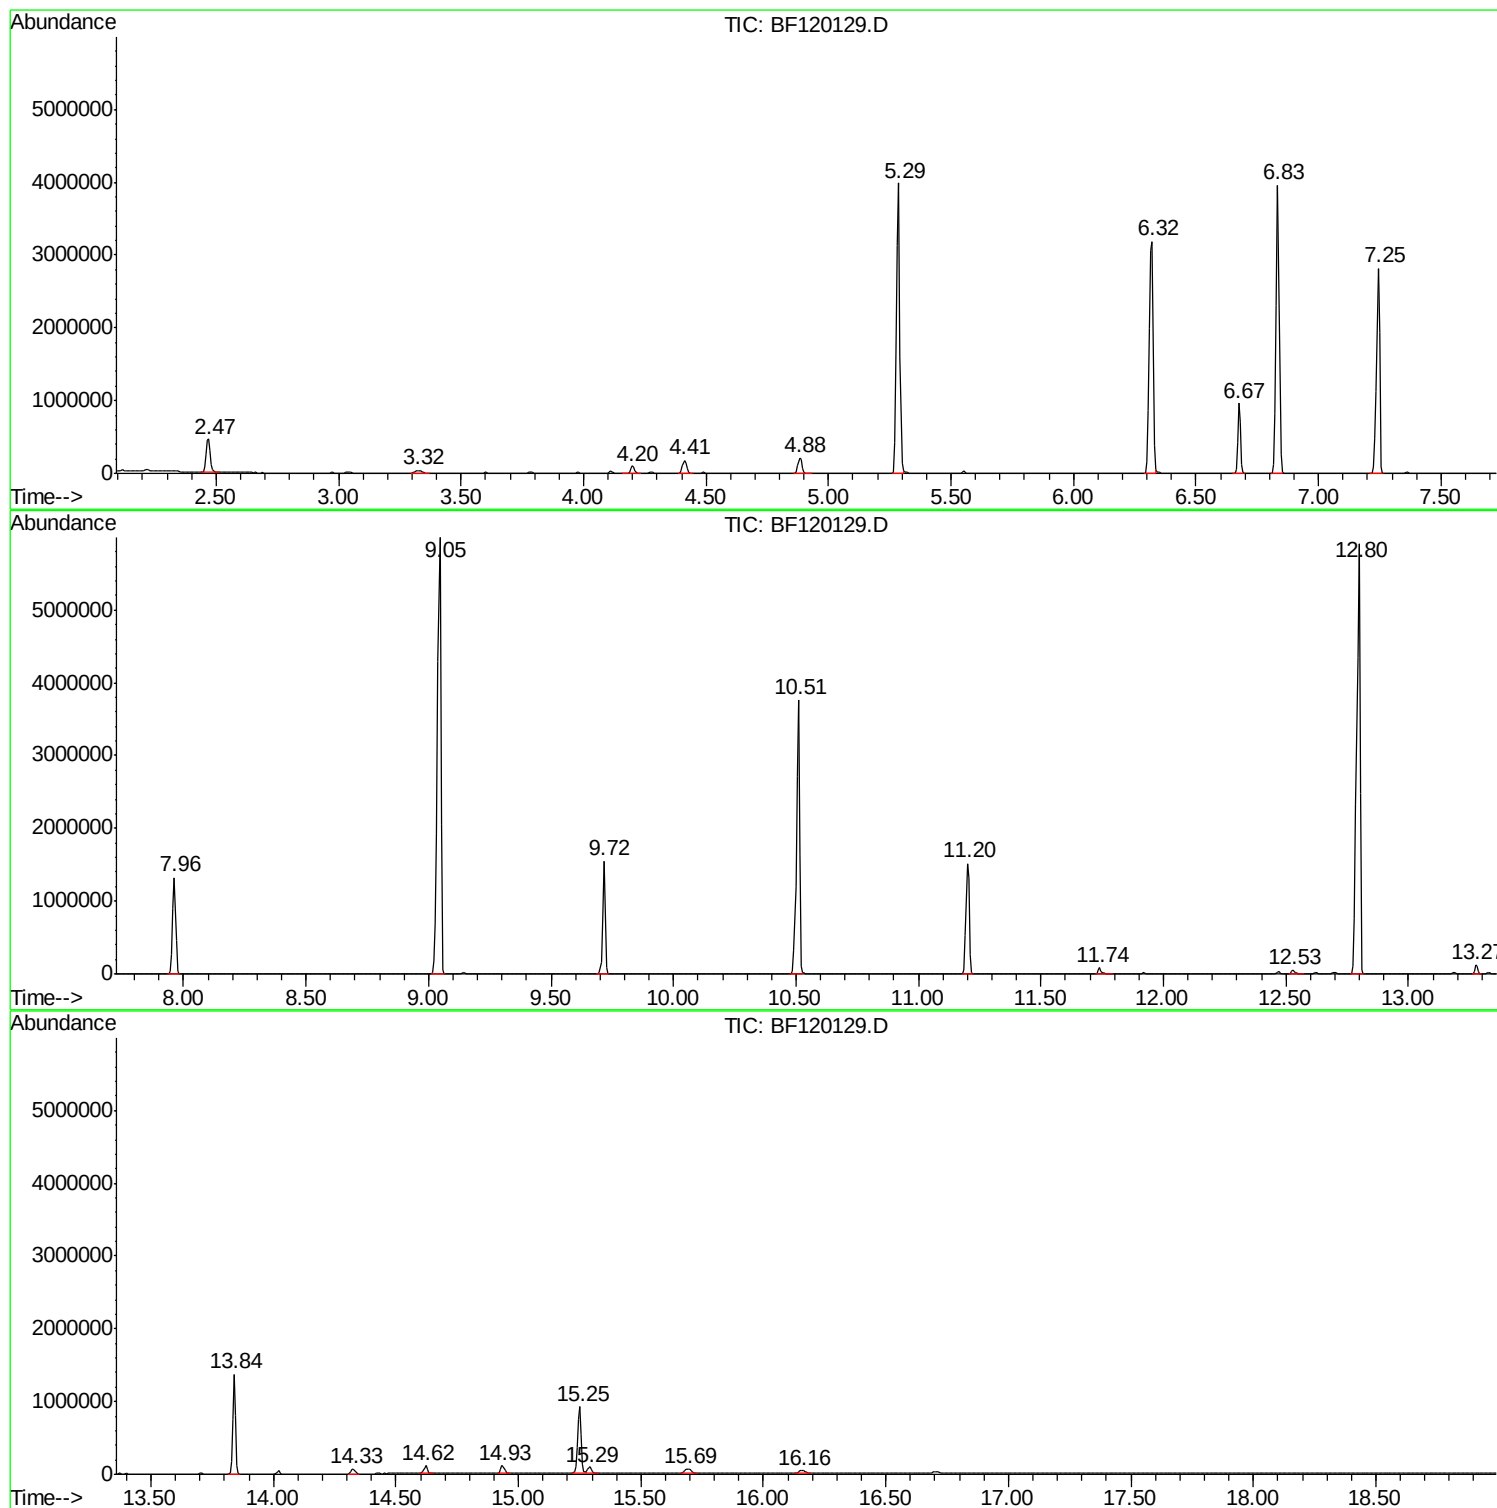

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120129.D
Acq On : 22 Apr 2020 14:20
Operator : MA/SJ
Sample : L2327-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
Data File : BF120129.D
Acq On : 22 Apr 2020 14:20
Operator : MA/SJ
Sample : L2327-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-4-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc