

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042220\
 Data File : BF120130.D
 Acq On : 22 Apr 2020 14:50
 Operator : MA/SJ
 Sample : PB128411BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128411BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.281	538	543	546	rBV	4348219	4423574	79.70%	12.366%
2	6.322	714	720	723	rBV	3972842	4280480	77.12%	11.966%
3	6.675	777	780	784	rBV	961670	785674	14.15%	2.196%
4	6.834	802	807	810	rBV	4054339	3546765	63.90%	9.915%
5	7.245	871	877	880	rBV	2867082	2933281	52.85%	8.200%
6	7.963	995	999	1002	rBV	1278656	1047487	18.87%	2.928%
7	9.045	1177	1183	1186	rBV	5888996	5250442	94.59%	14.677%
8	9.716	1293	1297	1300	rBV	1497651	1191024	21.46%	3.329%
9	10.510	1427	1432	1435	rBV	3613998	3351100	60.37%	9.368%
10	11.204	1546	1550	1553	rBV	1382897	1255863	22.63%	3.511%
11	12.798	1816	1821	1824	rBV	5487995	5550519	100.00%	15.516%
12	13.839	1994	1998	2002	rBV	1303068	1144951	20.63%	3.201%
13	15.251	2233	2238	2242	rBV	891587	1011203	18.22%	2.827%


Sum of corrected areas: 35772363

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF042220\
Data File : BF120130.D
Acq On : 22 Apr 2020 14:50
Operator : MA/SJ
Sample : PB128411BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128411BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

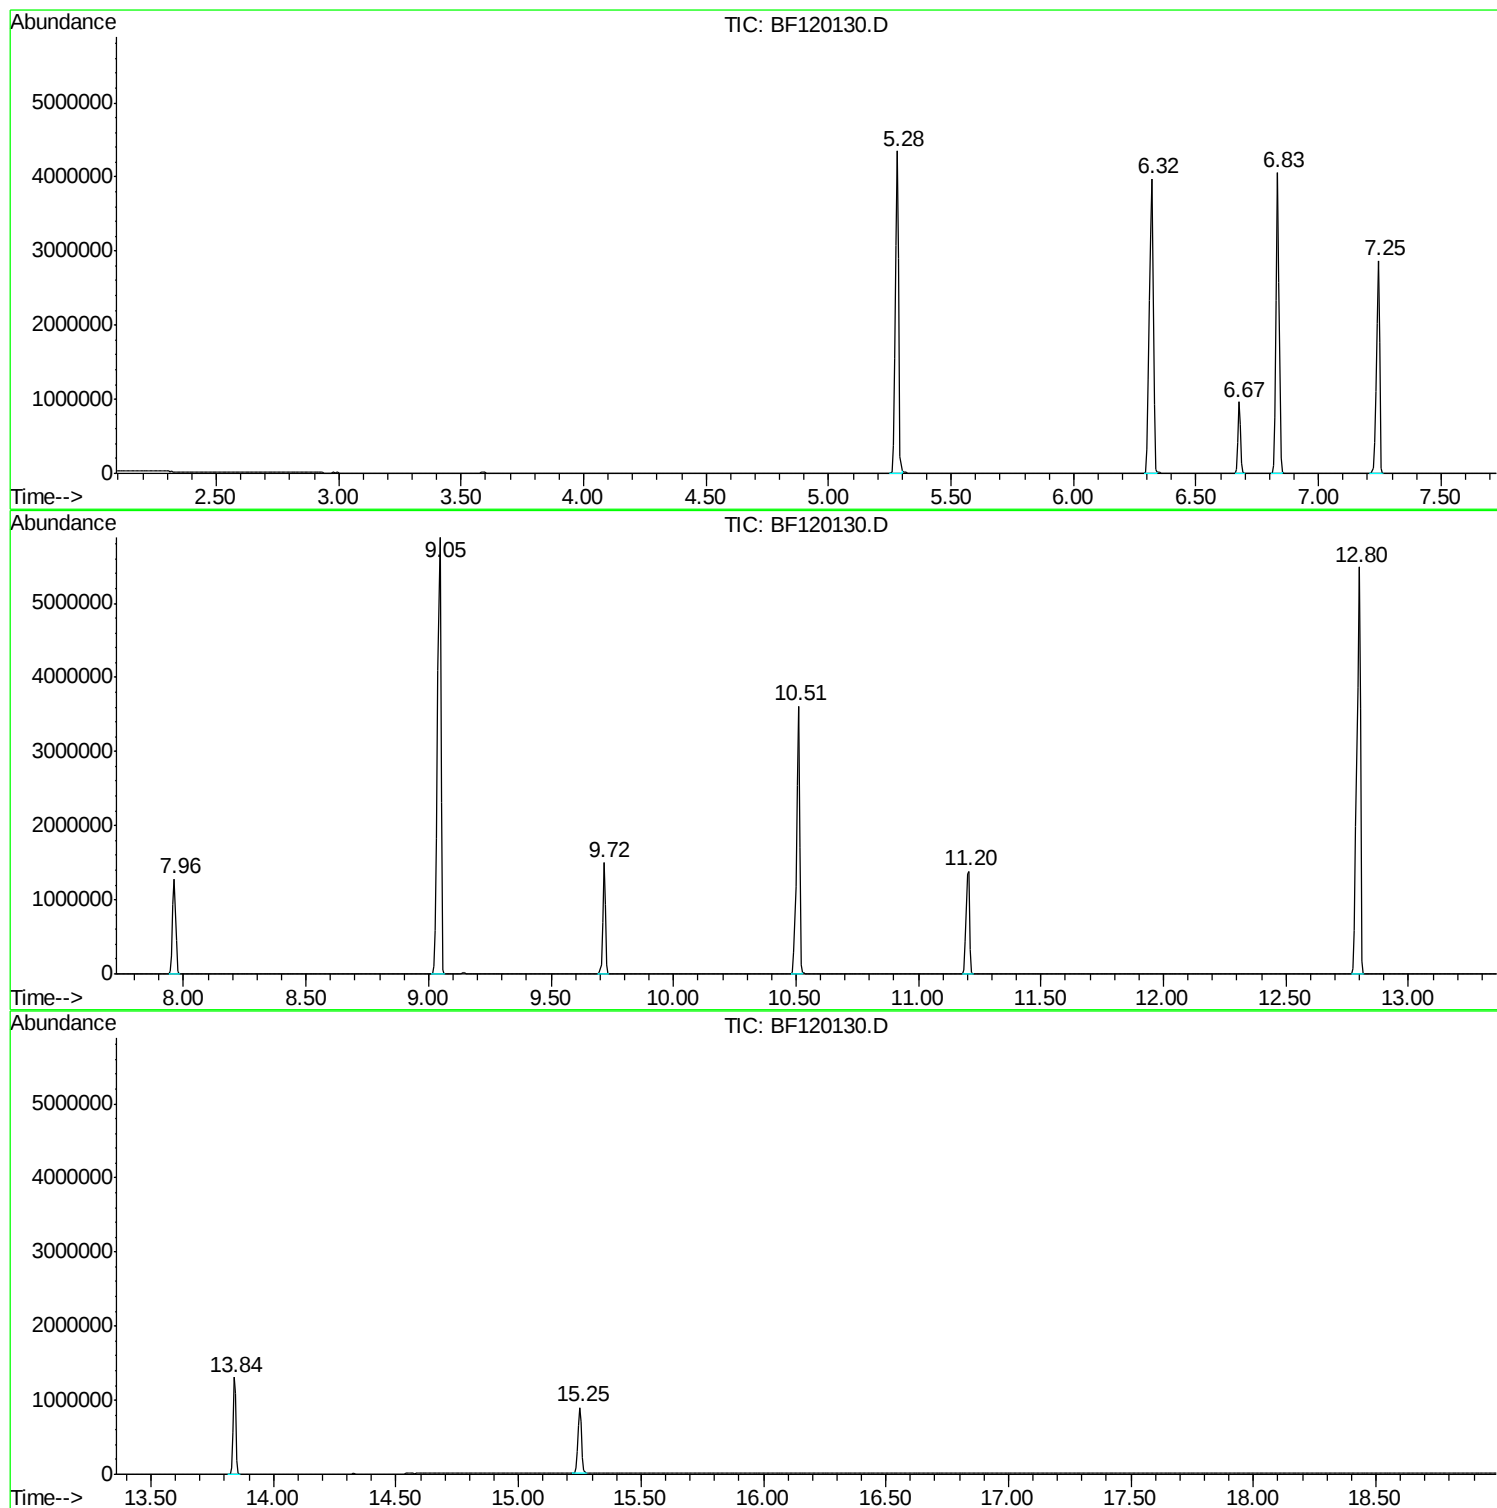

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042220\
Data File : BF120130.D
Acq On : 22 Apr 2020 14:50
Operator : MA/SJ
Sample : PB128411BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128411BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042220\
Data File : BF120130.D
Acq On : 22 Apr 2020 14:50
Operator : MA/SJ
Sample : PB128411BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128411BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc