


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042220\
 Data File : BF120121.D
 Acq On : 22 Apr 2020 10:44
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 13:31:01 2020

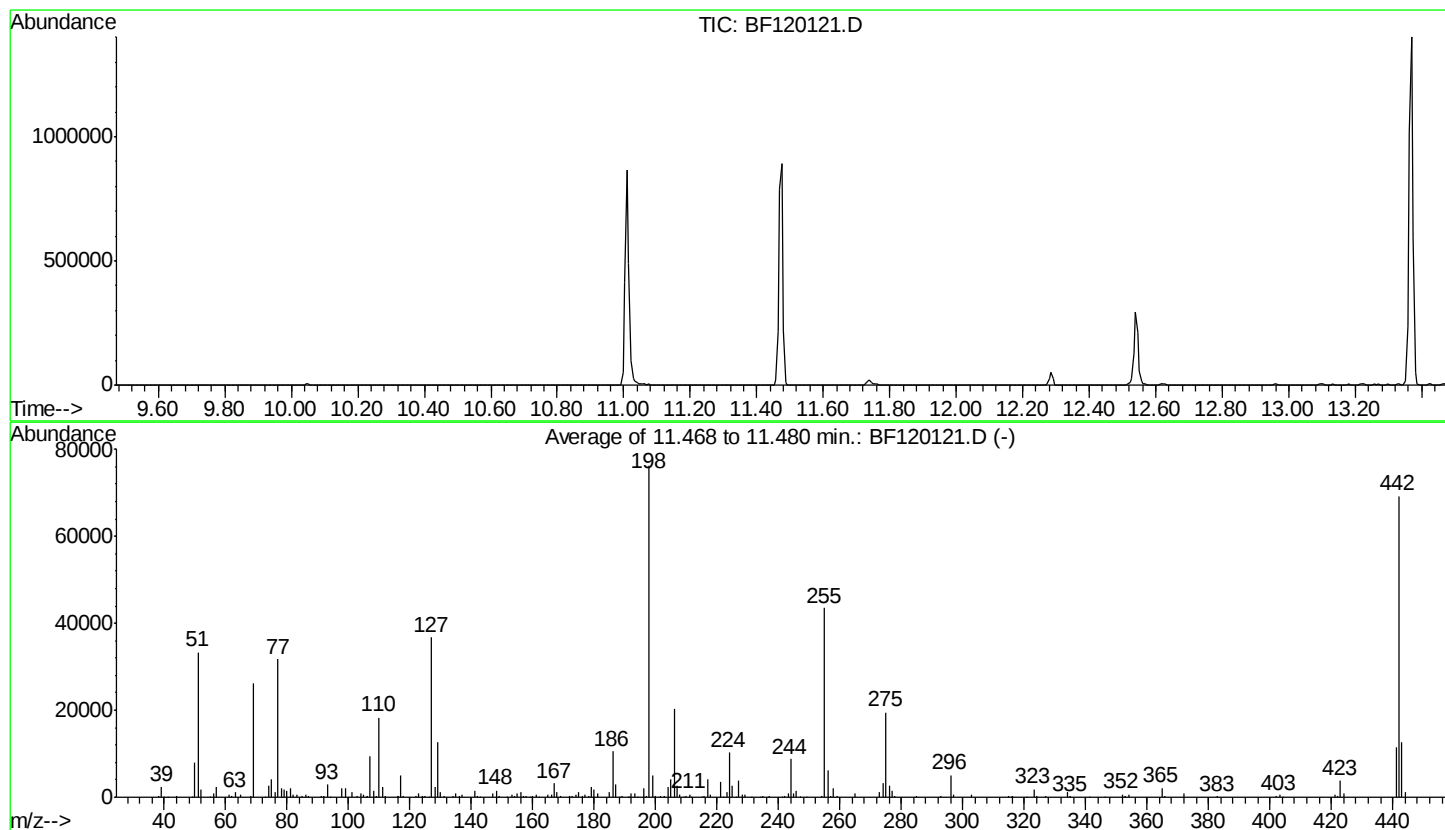

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	33357	PASS
68	69	0.00	2	1.5	386	PASS
69	198	0.00	100	34.3	26129	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	36687	PASS
197	198	0.00	2	0.6	424	PASS
198	198	100	100	100.0	76245	PASS
199	198	5	9	6.6	5005	PASS
275	198	10	60	25.5	19456	PASS
365	198	1	100	2.8	2120	PASS
441	198	0.01	100	14.9	11350	PASS
442	198	50	100	90.8	69197	PASS
443	442	15	24	18.4	12747	PASS