


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042220\
 Data File : BF120146.D
 Acq On : 23 Apr 2020 00:51
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 13:31:01 2020

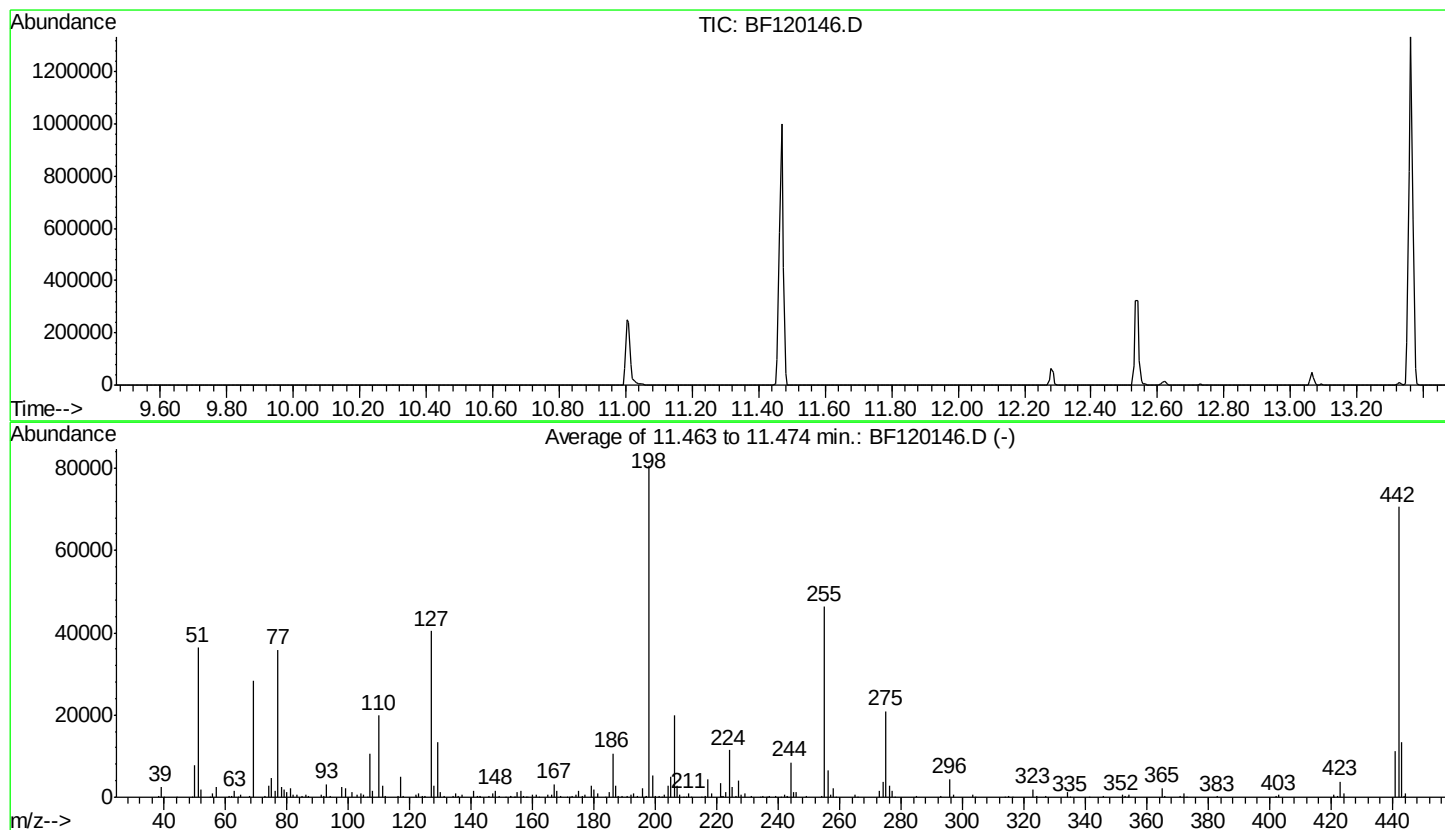

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	36403	PASS
68	69	0.00	2	1.5	414	PASS
69	198	0.00	100	35.3	28475	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	40461	PASS
197	198	0.00	2	0.6	469	PASS
198	198	100	100	100.0	80658	PASS
199	198	5	9	6.6	5289	PASS
275	198	10	60	26.0	20962	PASS
365	198	1	100	2.8	2271	PASS
441	198	0.01	100	14.1	11334	PASS
442	198	50	100	87.6	70653	PASS
443	442	15	24	19.1	13503	PASS