

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
 Data File : BF120171.D
 Acq On : 23 Apr 2020 18:45
 Operator : MA/SJ
 Sample : L2330-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-GW-2020-04-16

Quant Time: Apr 24 02:08:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 23 13:31:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	140202	20.00	ng	0.00
21) Naphthalene-d8	7.95	136	542366	20.00	ng	0.00
39) Acenaphthene-d10	9.70	164	298859	20.00	ng	0.00
64) Phenanthrene-d10	11.18	188	596313	20.00	ng	0.00
76) Chrysene-d12	13.82	240	481221	20.00	ng	-0.01
87) Perylene-d12	15.22	264	405374	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	505887	62.36	ng	0.00
7) Phenol-d6	6.30	99	404102	38.66	ng	-0.01
23) Nitrobenzene-d5	7.23	82	983529	93.81	ng	0.00
42) 2,4,6-Tribromophenol	10.49	330	472945	129.25	ng	0.00
45) 2-Fluorobiphenyl	9.03	172	1974099	93.78	ng	0.00
79) Terphenyl-d14	12.78	244	2488114	87.00	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120171.D
Acq On : 23 Apr 2020 18:45
Operator : MA/SJ
Sample : L2330-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-GW-2020-04-16

Quant Time: Apr 24 02:08:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 13:31:01 2020
Response via : Initial Calibration

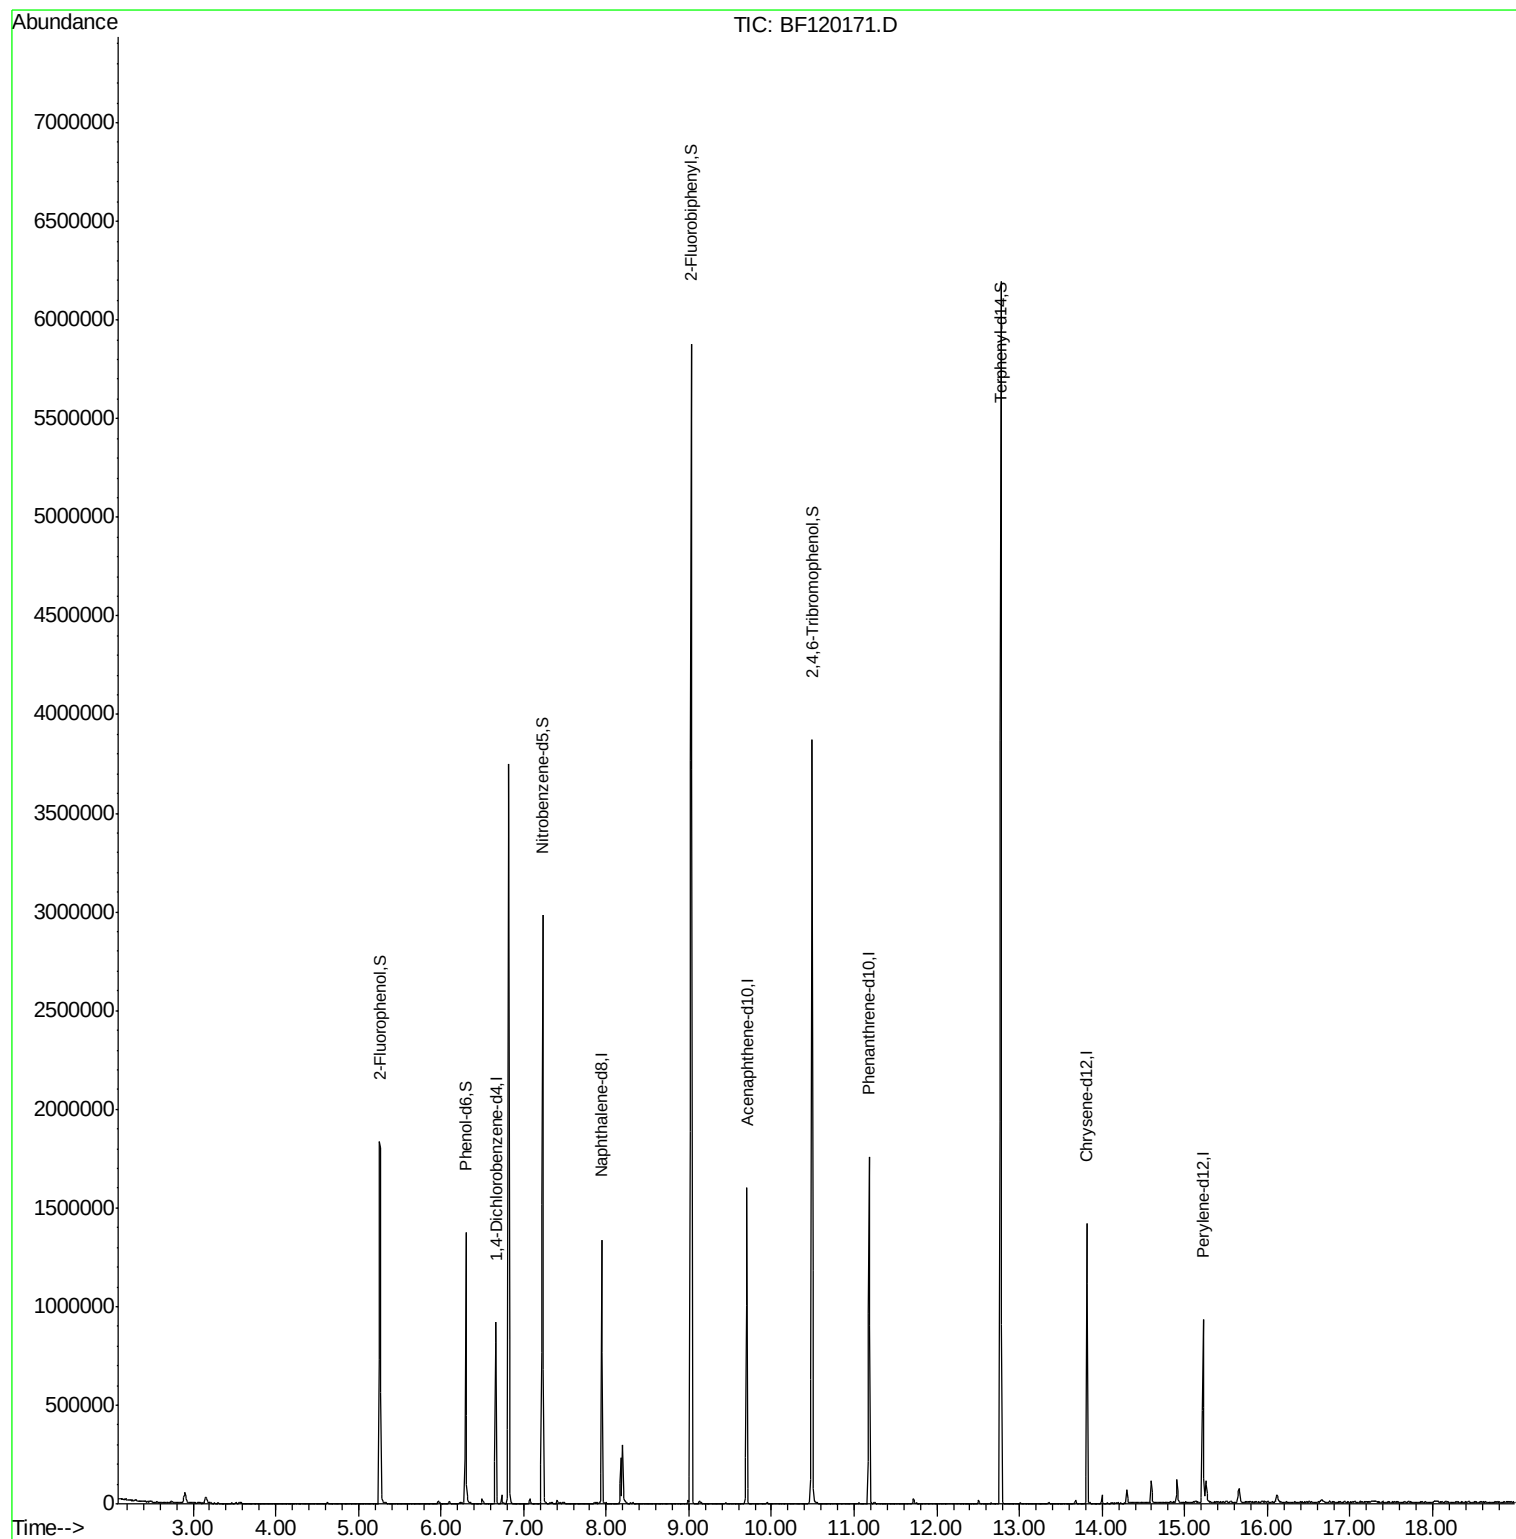

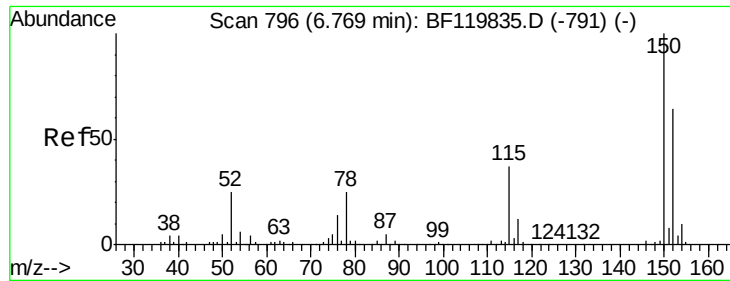


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.66 min Scan# 778
Delta R.T. -0.00 min
Lab File: BF120171.D
Acq: 23 Apr 2020 18:45

Instrument :
BNA_F
ClientSampleId :
FB-GW-2020-04-16

Tgt Ion:152 Resp: 140202
Ion Ratio Lower Upper
152 100
150 152.8 124.5 186.7
115 56.1 49.6 74.4

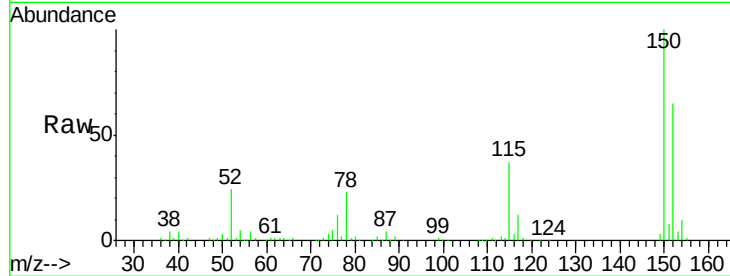


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

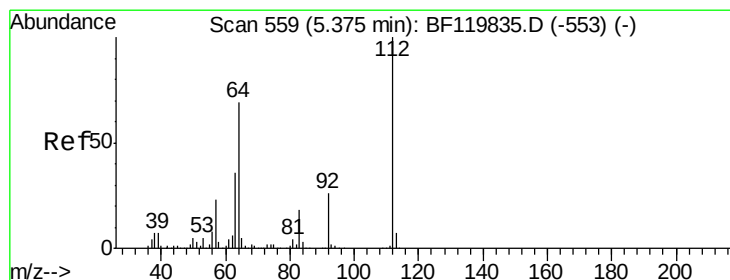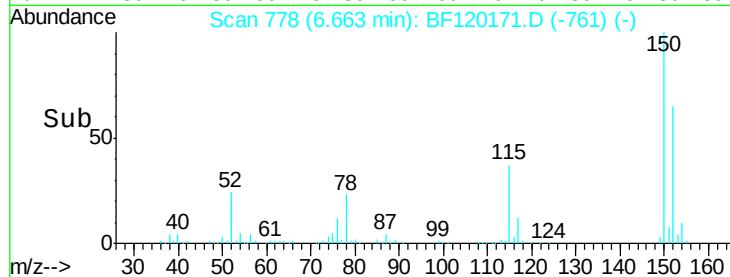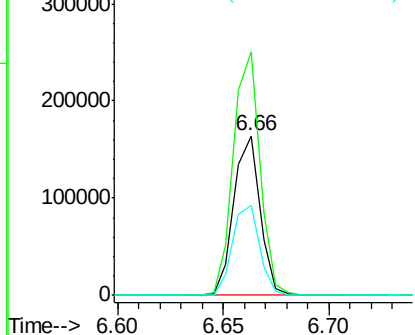



#5


2-Fluorophenol
Concen: 62.36 ng
RT: 5.26 min Scan# 540
Delta R.T. -0.00 min
Lab File: BF120171.D
Acq: 23 Apr 2020 18:45

Tgt Ion:112 Resp: 505887
Ion Ratio Lower Upper
112 100
64 64.3 56.7 85.1
63 33.7 29.5 44.3

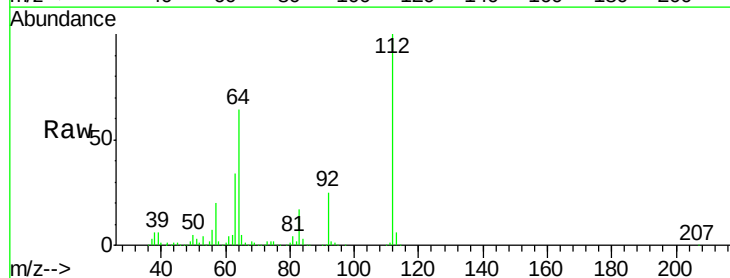

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

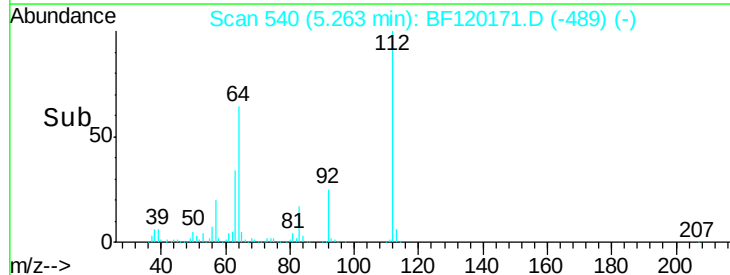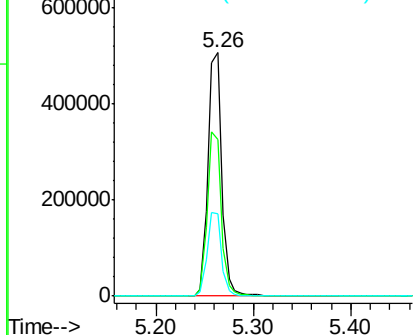

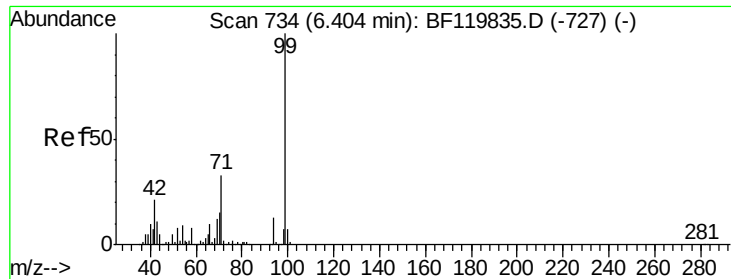

#7

Phenol-d6

Concen: 38.66 ng

RT: 6.30 min Scan# 716

Delta R.T. -0.01 min

Lab File: BF120171.D

Acq: 23 Apr 2020 18:45

Instrument :

BNA_F

ClientSampleId :

FB-GW-2020-04-16





Tgt Ion: 99 Resp: 404102

Ion Ratio Lower Upper

99 100

42 19.3 16.6 24.8

71 31.3 26.4 39.6

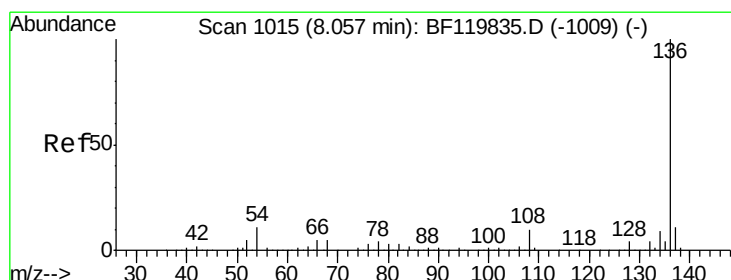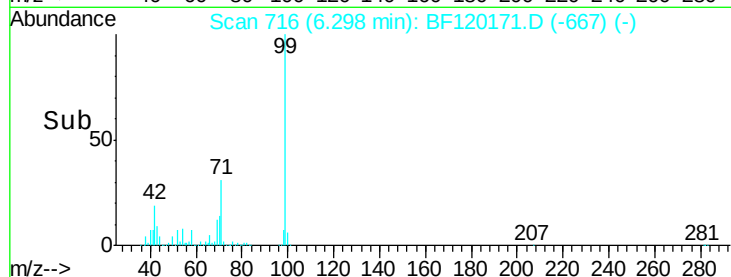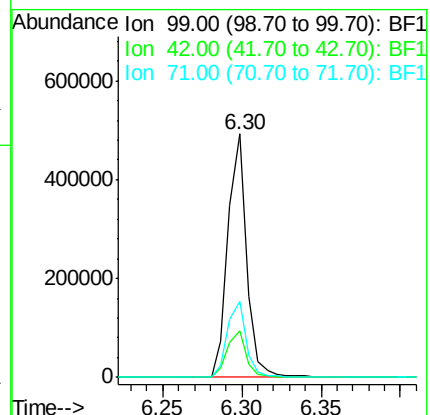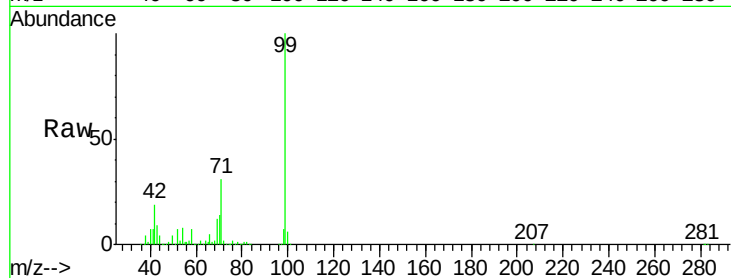

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 996

Delta R.T. -0.01 min

Lab File: BF120171.D

Acq: 23 Apr 2020 18:45

Tgt Ion: 136 Resp: 542366




Ion Ratio Lower Upper


136 100

137 11.2 8.7 13.1

54 10.5 9.1 13.7

68 5.5 4.6 6.8

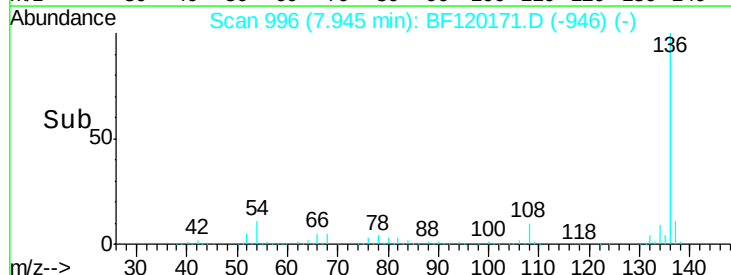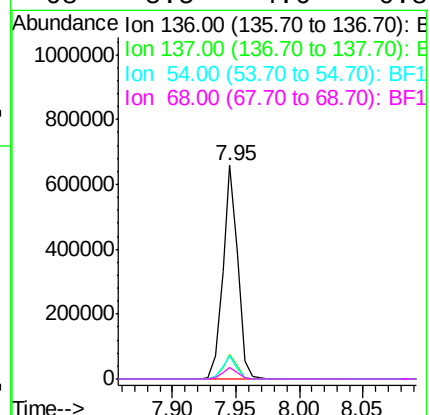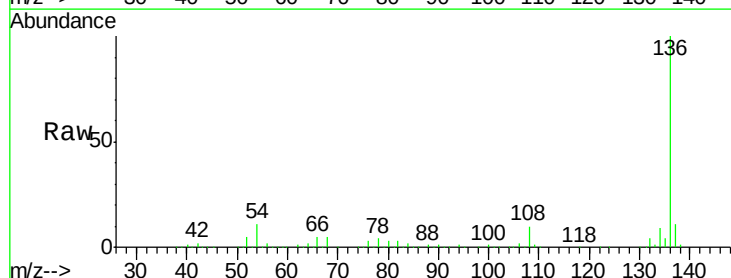


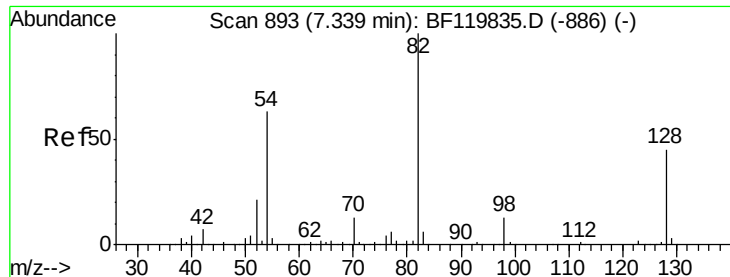




#23
 Nitrobenzene-d5
 Concen: 93.81 ng
 RT: 7.23 min Scan# 875
 Delta R.T. -0.01 min
 Lab File: BF120171.D
 Acq: 23 Apr 2020 18:45

Instrument :
 BNA_F
 ClientSampleId :
 FB-GW-2020-04-16

Tgt Ion: 82 Resp: 983529
 Ion Ratio Lower Upper
 82 100
 128 46.3 36.3 54.5
 54 60.9 50.6 75.8

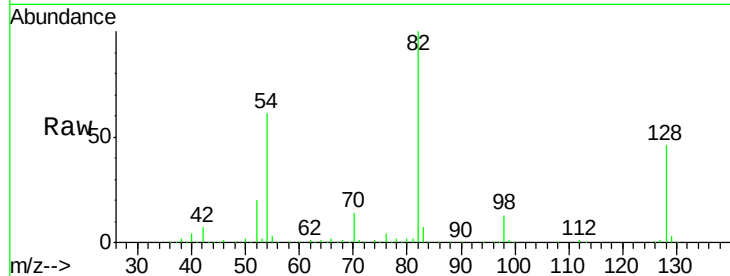


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

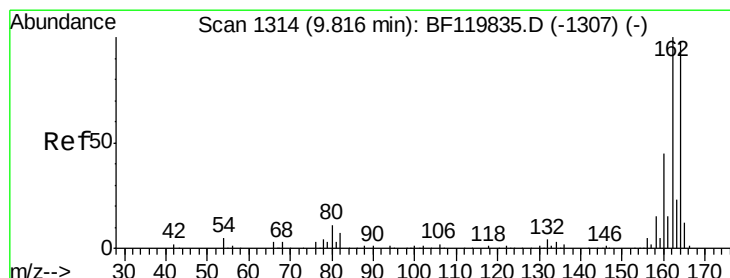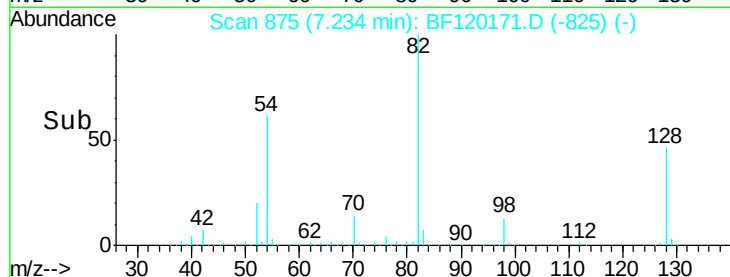
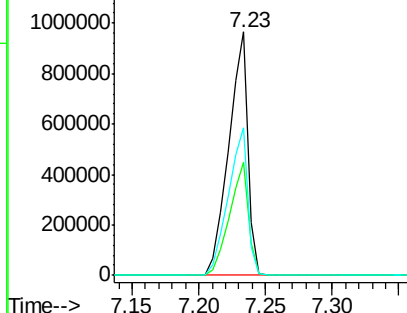



#39
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.70 min Scan# 1294
 Delta R.T. -0.01 min
 Lab File: BF120171.D
 Acq: 23 Apr 2020 18:45

Tgt Ion: 164 Resp: 298859
 Ion Ratio Lower Upper
 164 100
 162 101.9 80.6 121.0
 160 44.5 35.7 53.5

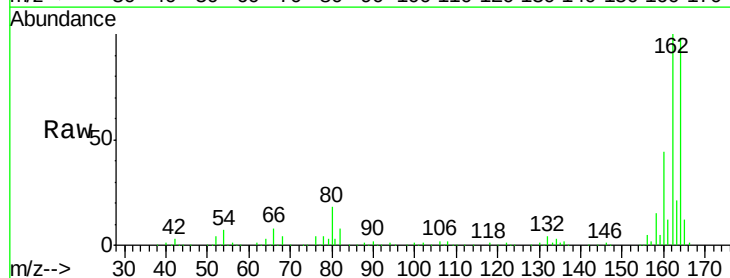

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

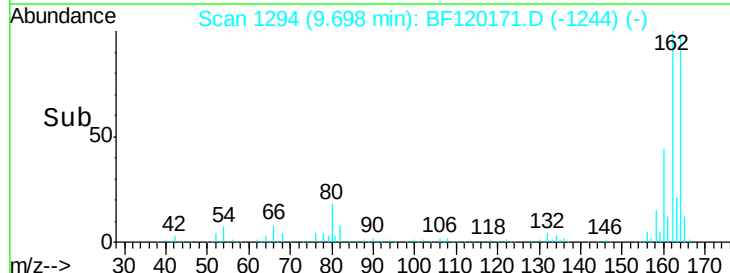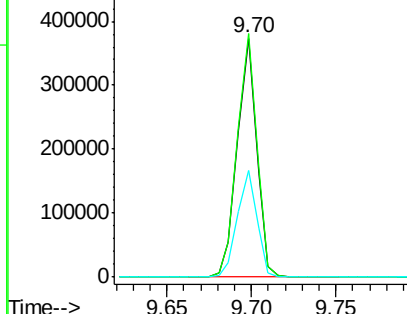

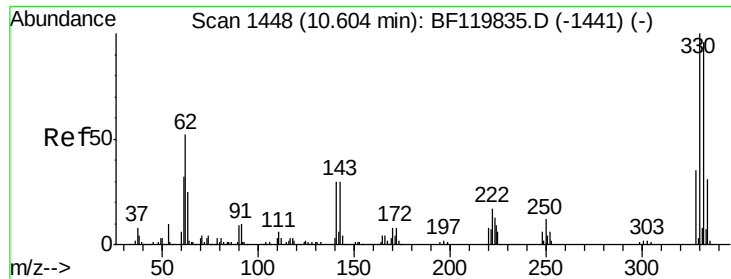

#42

2,4,6-Tribromophenol

Concen: 129.25 ng

RT: 10.49 min Scan# 1429

Delta R.T. -0.00 min

Lab File: BF120171.D

Acq: 23 Apr 2020 18:45

Instrument :

BNA_F

ClientSampleId :

FB-GW-2020-04-16


Tgt Ion:330 Resp: 472945

Ion Ratio Lower Upper

330 100

332 98.0 75.7 113.5




141 34.9 25.4 38.0

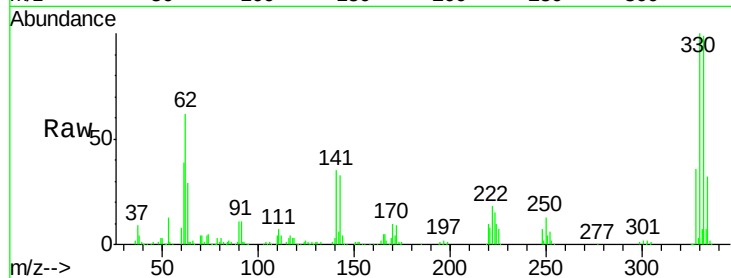

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

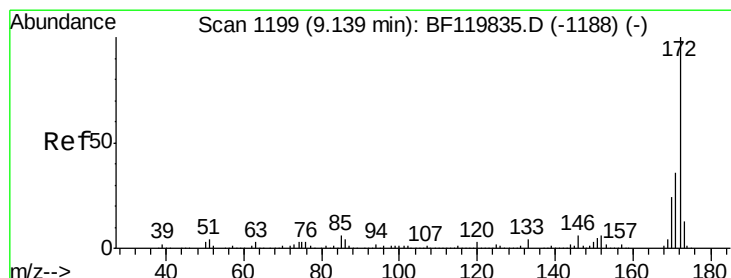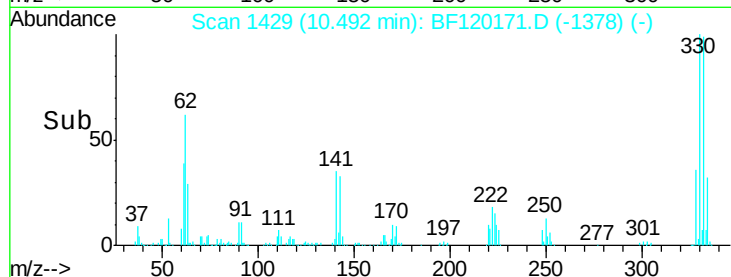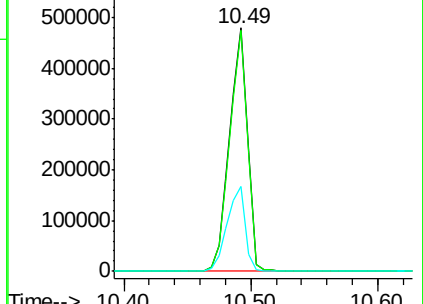

#45

2-Fluorobiphenyl

Concen: 93.78 ng

RT: 9.03 min Scan# 1180

Delta R.T. -0.01 min

Lab File: BF120171.D

Acq: 23 Apr 2020 18:45


Tgt Ion:172 Resp: 1974099

Ion Ratio Lower Upper

172 100

171 36.1 29.6 44.4



170 24.0 20.2 30.2

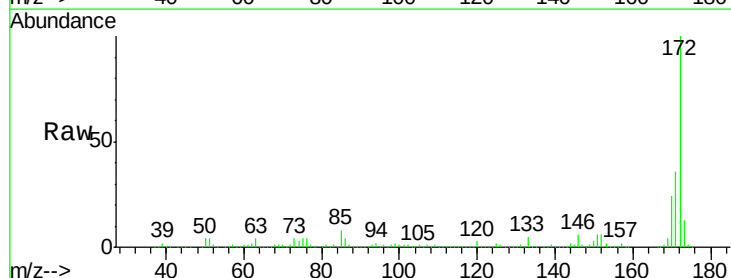


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



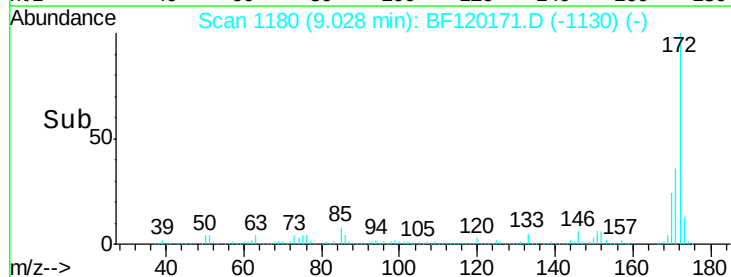
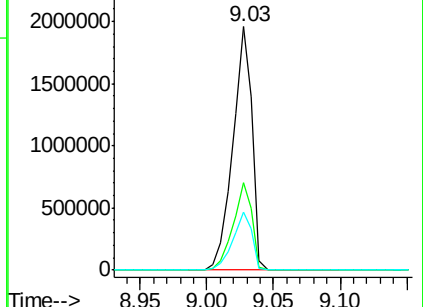


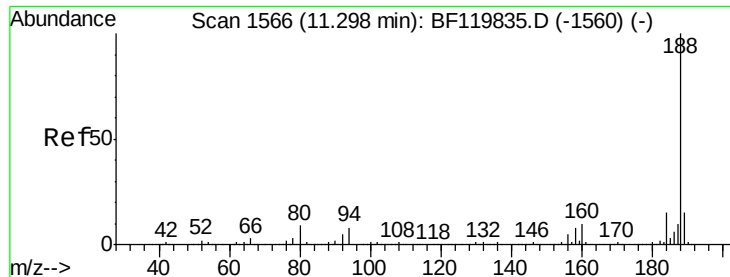

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.18 min Scan# 1546
Delta R.T. -0.01 min
Lab File: BF120171.D
Acq: 23 Apr 2020 18:45




Instrument :
BNA_F
ClientSampleId :
FB-GW-2020-04-16


Tgt Ion	Ratio	Resp	Lower	Upper
188	100	596313		
94	9.1	7.5	11.3	
80	9.3	9.0	13.4	

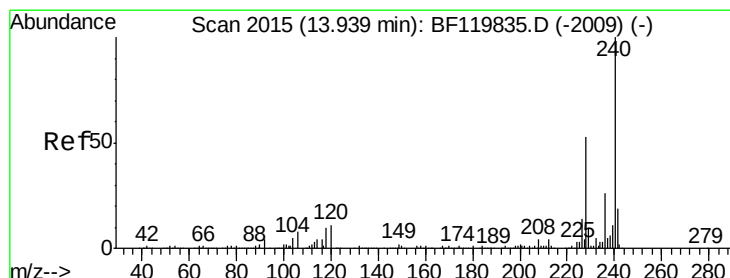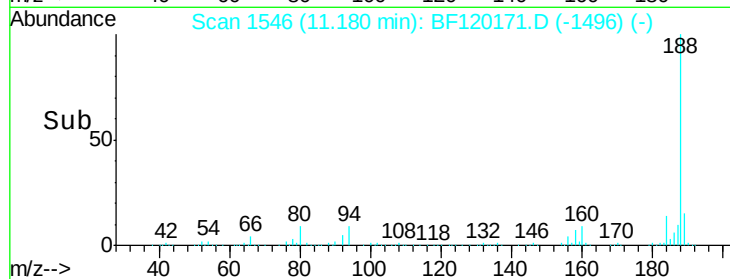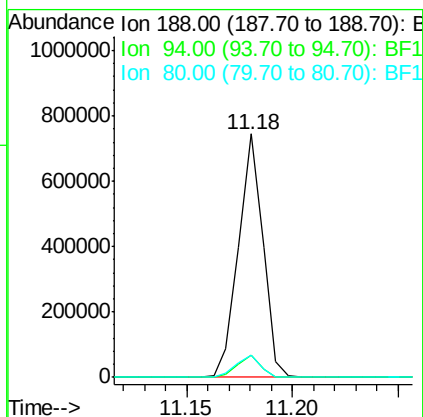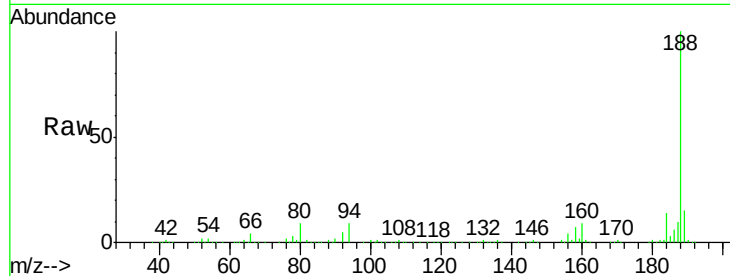

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.82 min Scan# 1994
Delta R.T. -0.01 min
Lab File: BF120171.D
Acq: 23 Apr 2020 18:45

Tgt Ion	Ratio	Resp	Lower	Upper
240	100	481221		
120	11.7	10.6	15.8	
236	26.0	20.2	30.2	

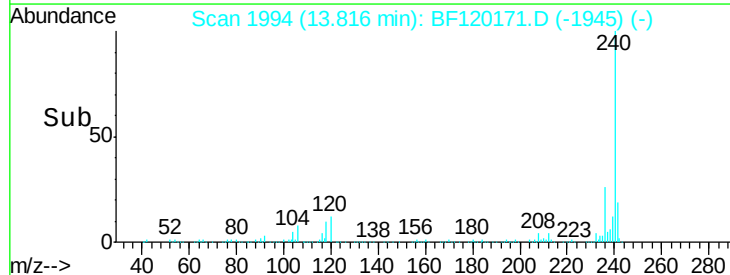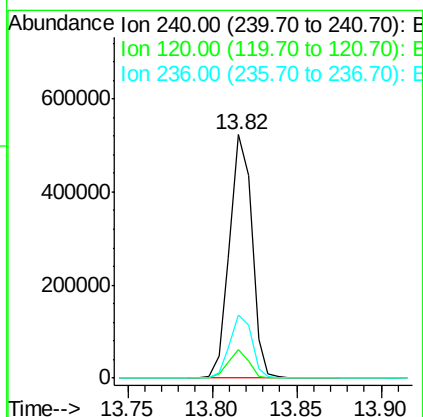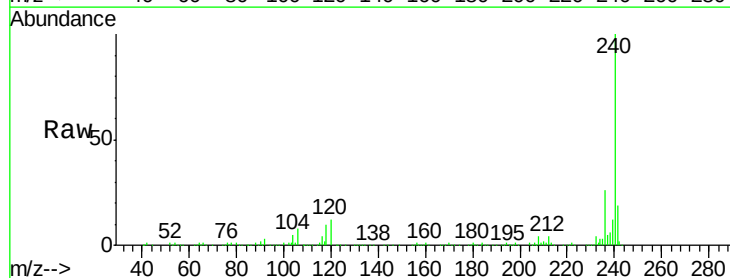

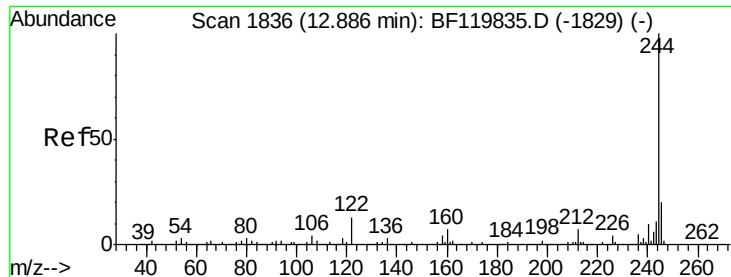

#79

Terphenyl-d14

Concen: 87.00 ng

RT: 12.78 min Scan# 1818

Delta R.T. 0.01 min

Lab File: BF120171.D

Acq: 23 Apr 2020 18:45

Instrument :

BNA_F

ClientSampleId :

FB-GW-2020-04-16


Tgt Ion:244 Resp: 2488114

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8




122 12.5 10.3 15.5

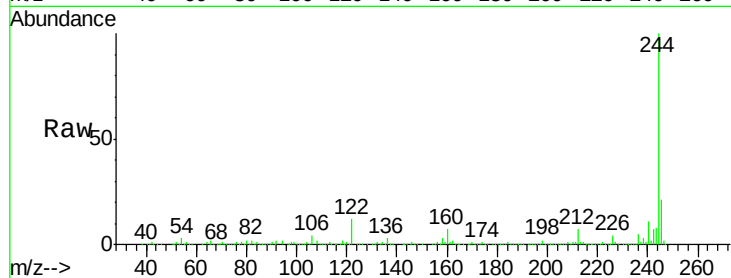

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

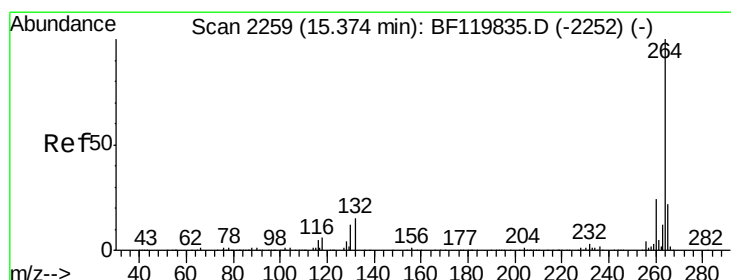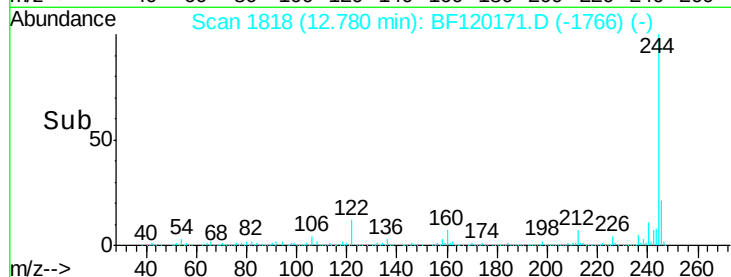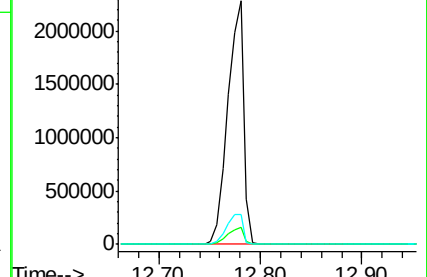

#87

Perylene-d12

Concen: 20.00 ng

RT: 15.22 min Scan# 2233

Delta R.T. -0.01 min

Lab File: BF120171.D

Acq: 23 Apr 2020 18:45


Tgt Ion:264 Resp: 405374

Ion Ratio Lower Upper

264 100

260 24.6 18.7 28.1

265 21.8 17.7 26.5

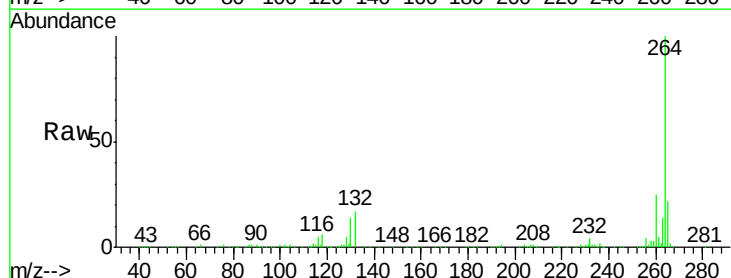

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

