

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
 Data File : BF120160.D
 Acq On : 23 Apr 2020 13:49
 Operator : MA/SJ
 Sample : PB128435BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128435BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	543	rBV	3800038	4029838	69.53%	11.479%
2	6.304	712	717	720	rBV	3482987	4001406	69.04%	11.398%
3	6.663	774	778	789	rVB	928858	773870	13.35%	2.204%
4	6.822	800	805	808	rBV	3557309	3300329	56.95%	9.401%
5	7.234	869	875	877	rBV	2479490	2719772	46.93%	7.747%
6	7.945	992	996	999	rBV	1282044	1022233	17.64%	2.912%
7	9.028	1174	1180	1183	rBV	5588826	5090582	87.84%	14.500%
8	9.698	1289	1294	1297	rBV	1567448	1236046	21.33%	3.521%
9	10.492	1423	1429	1432	rBV	3506942	3433666	59.25%	9.780%
10	11.180	1542	1546	1549	rBV	1779869	1353954	23.36%	3.857%
11	12.780	1812	1818	1820	rBV	5115731	5795419	100.00%	16.508%
12	13.815	1990	1994	1998	rBV	1310009	1214753	20.96%	3.460%
13	15.221	2228	2233	2238	rBV	974329	1135751	19.60%	3.235%


Sum of corrected areas: 35107619

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120160.D
Acq On : 23 Apr 2020 13:49
Operator : MA/SJ
Sample : PB128435BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128435BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

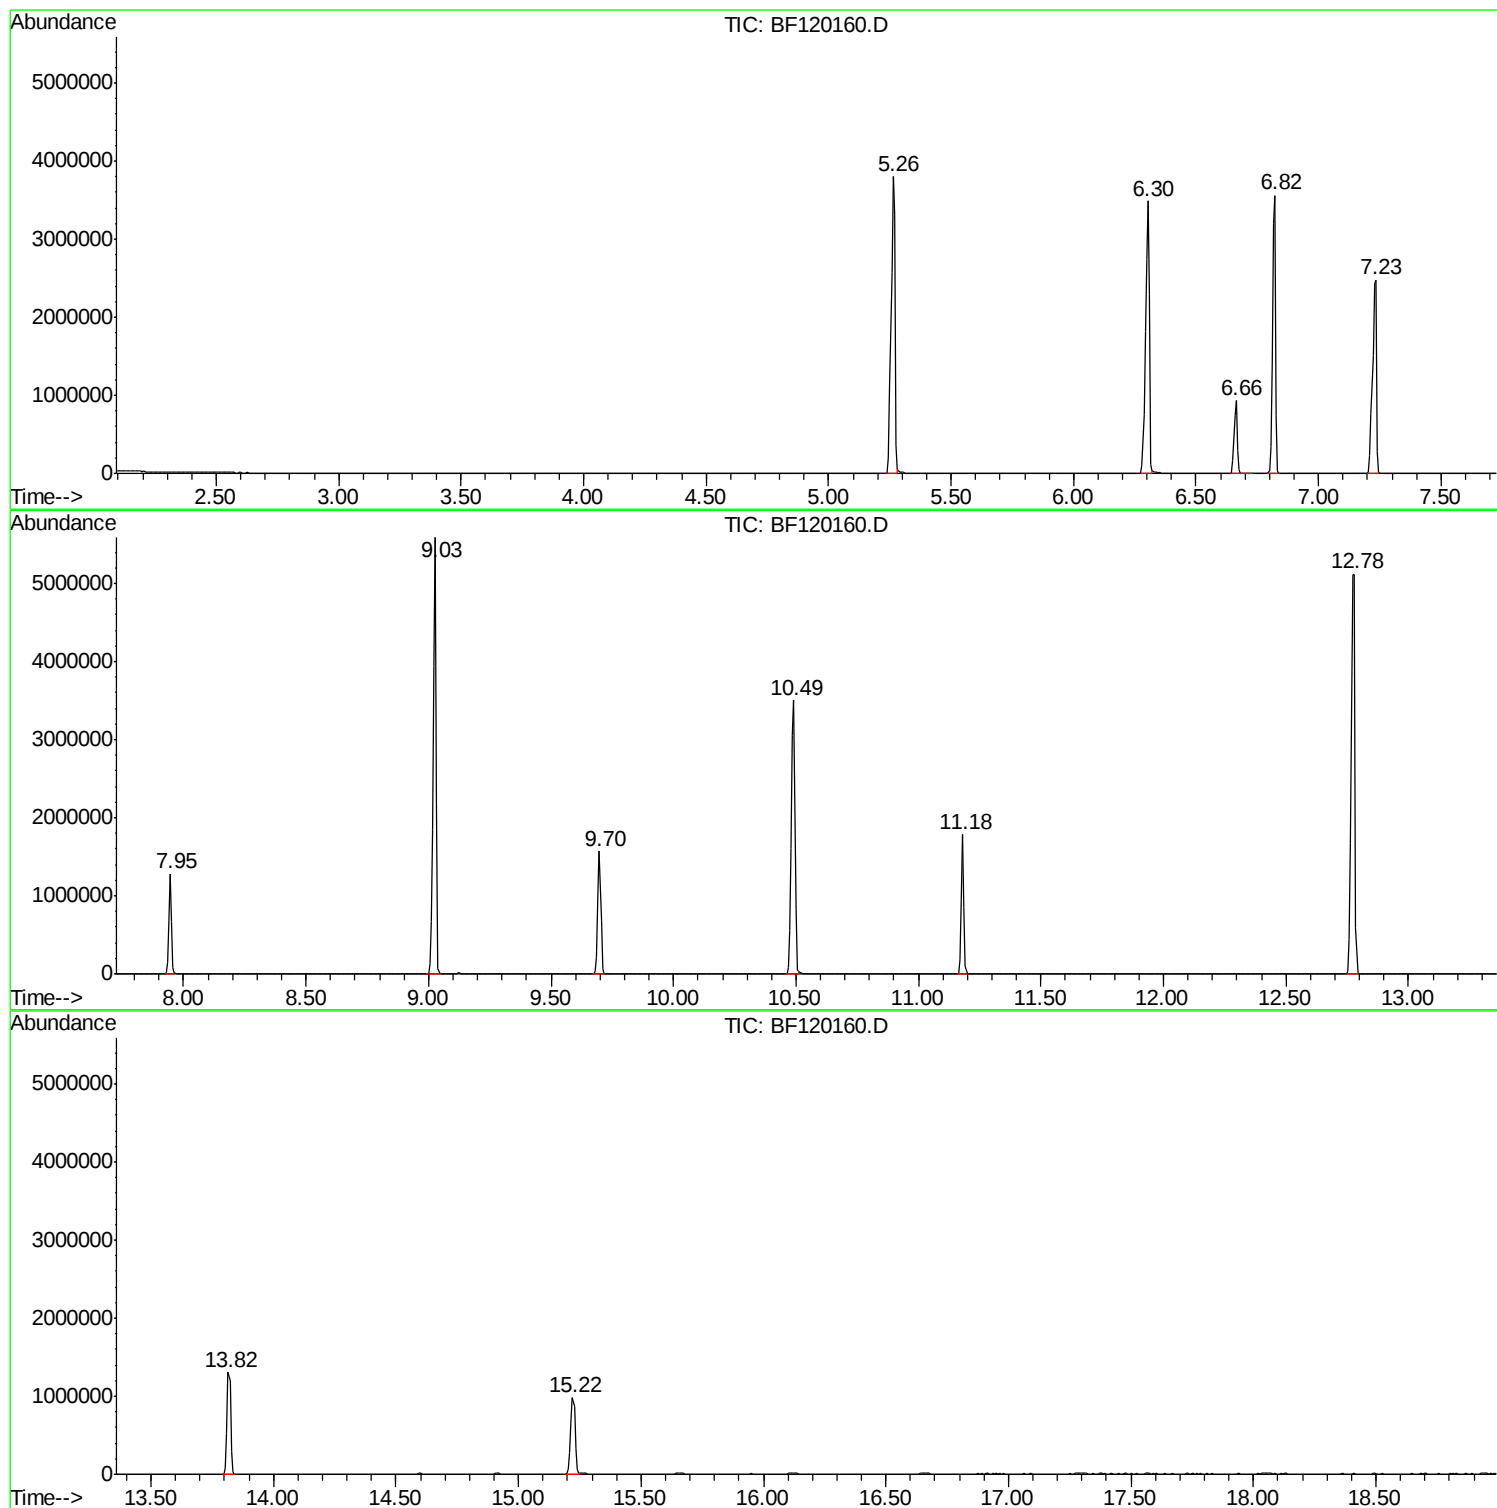

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120160.D
Acq On : 23 Apr 2020 13:49
Operator : MA/SJ
Sample : PB128435BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128435BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120160.D
Acq On : 23 Apr 2020 13:49
Operator : MA/SJ
Sample : PB128435BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128435BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc