

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
 Data File : BF120169.D
 Acq On : 23 Apr 2020 17:51
 Operator : MA/SJ
 Sample : L2330-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PA-TWP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	550	rBV	2882539	2690302	41.63%	7.873%
2	6.298	712	716	719	rBV	2164669	1795673	27.79%	5.255%
3	6.663	774	778	785	rBV	945694	834902	12.92%	2.443%
4	6.822	800	805	808	rBV	3715338	3577043	55.36%	10.468%
5	7.234	869	875	878	rBV	2925090	3020000	46.74%	8.838%
6	7.945	992	996	1000	rBV	1355840	1102121	17.06%	3.225%
7	9.028	1174	1180	1183	rBV	6081107	5719933	88.52%	16.739%
8	9.698	1290	1294	1297	rBV	1708359	1333426	20.64%	3.902%
9	10.492	1423	1429	1432	rBV	3791318	3761279	58.21%	11.007%
10	11.180	1542	1546	1549	rBV	1791165	1442153	22.32%	4.220%
11	12.780	1812	1818	1820	rBV	5618704	6461953	100.00%	18.911%
12	13.816	1990	1994	1998	rBV	1405489	1300592	20.13%	3.806%
13	15.221	2228	2233	2237	rBV	1021085	1131553	17.51%	3.311%


Sum of corrected areas: 34170930

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120169.D
Acq On : 23 Apr 2020 17:51
Operator : MA/SJ
Sample : L2330-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

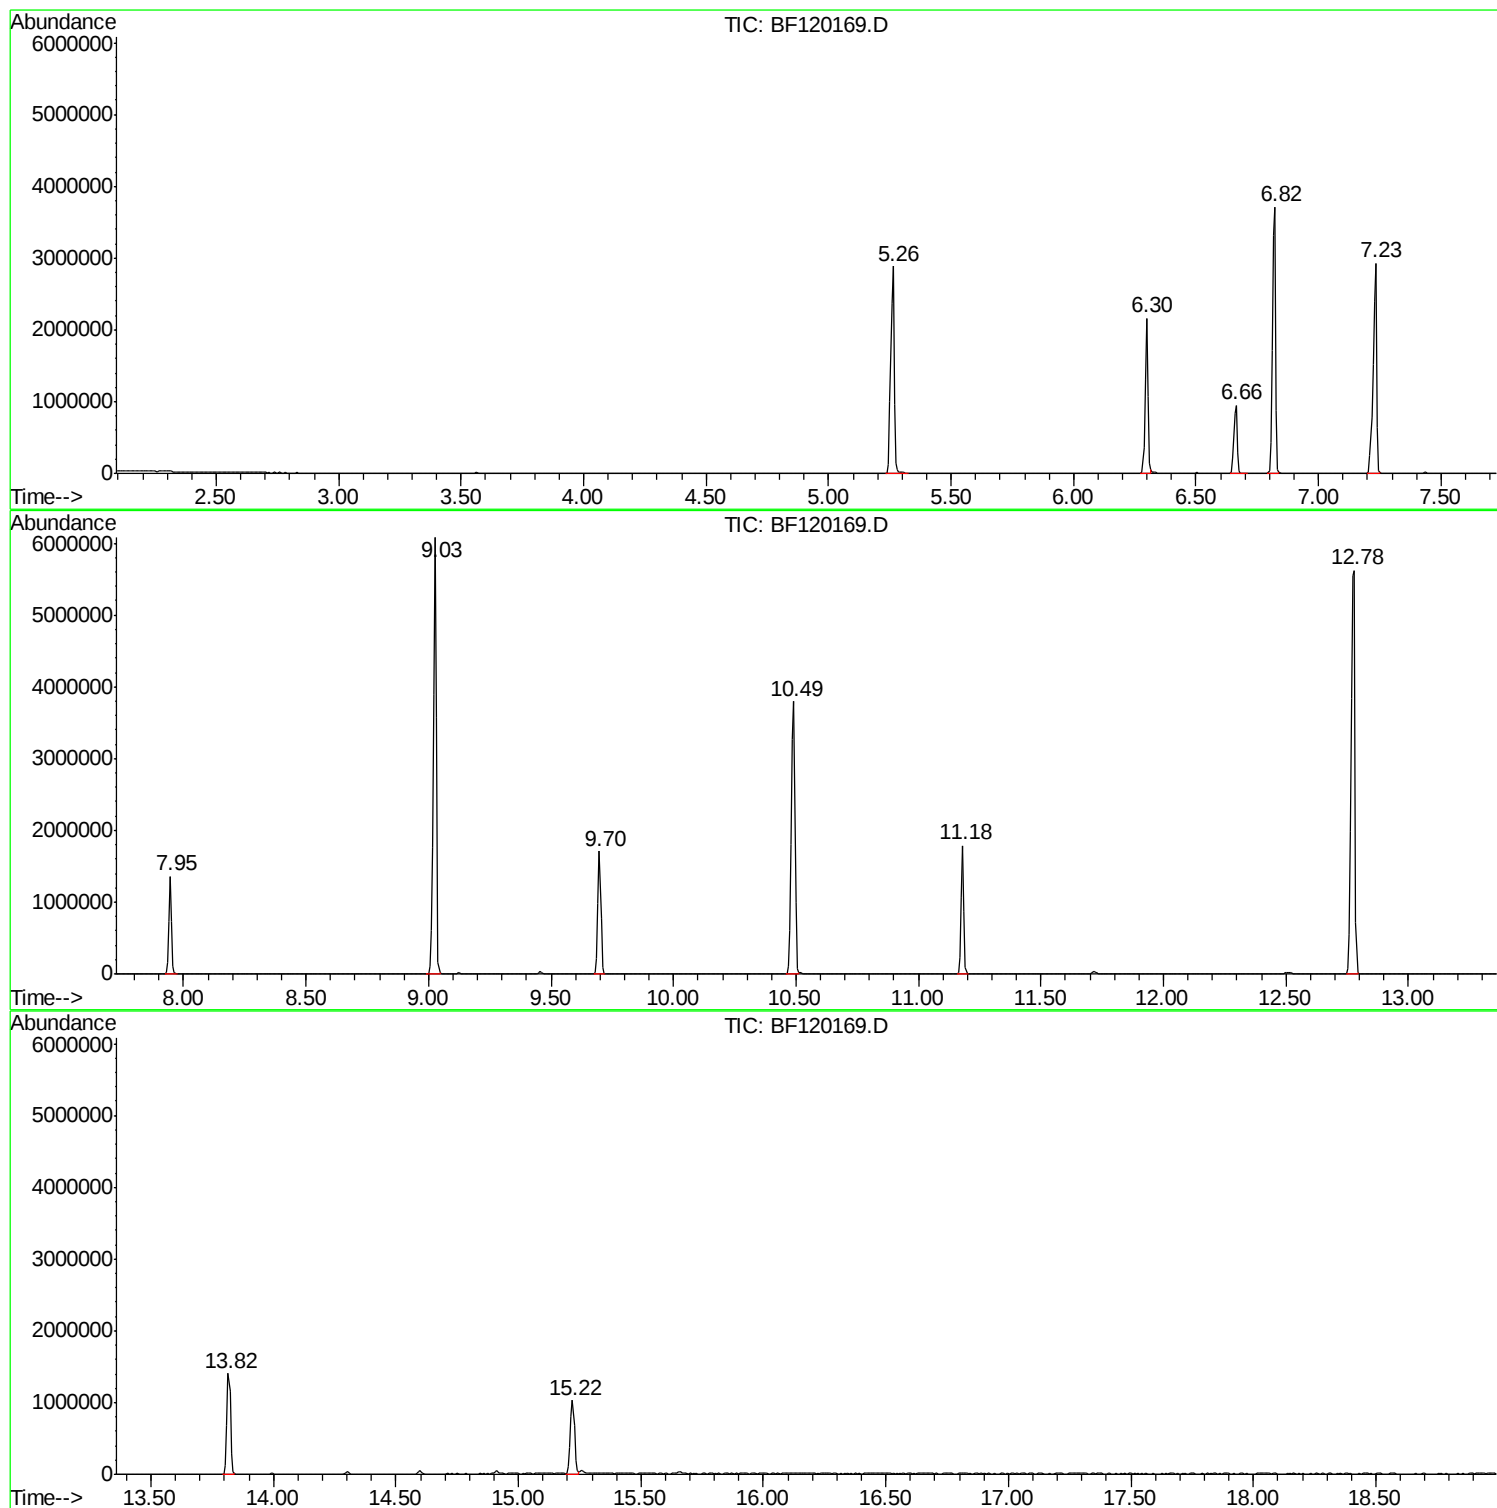

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120169.D
Acq On : 23 Apr 2020 17:51
Operator : MA/SJ
Sample : L2330-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120169.D
Acq On : 23 Apr 2020 17:51
Operator : MA/SJ
Sample : L2330-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc