

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120172.D
Acq On : 23 Apr 2020 19:12
Operator : MA/SJ
Sample : L2330-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	552	rBV	2510242	2429692	37.86%	7.368%
2	6.298	712	716	719	rBV	1877383	1554939	24.23%	4.715%
3	6.663	774	778	781	rBV	963517	835558	13.02%	2.534%
4	6.822	800	805	808	rBV	3774087	3577178	55.74%	10.848%
5	7.234	870	875	878	rVB	2967884	2968542	46.26%	9.002%
6	7.945	992	996	1000	rBV	1390167	1131202	17.63%	3.430%
7	9.028	1174	1180	1183	rBV	5600781	5293280	82.49%	16.052%
8	9.698	1289	1294	1297	rBV	1669054	1328998	20.71%	4.030%
9	10.492	1423	1429	1432	rBV	3626669	3538412	55.14%	10.730%
10	11.181	1542	1546	1549	rBV	1772663	1488352	23.19%	4.513%
11	12.780	1811	1818	1820	rBV	5652675	6417216	100.00%	19.460%
12	13.816	1990	1994	1998	rBV	1439310	1292742	20.14%	3.920%
13	15.221	2228	2233	2237	rBV	989082	1119652	17.45%	3.395%


Sum of corrected areas: 32975763

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120172.D
Acq On : 23 Apr 2020 19:12
Operator : MA/SJ
Sample : L2330-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

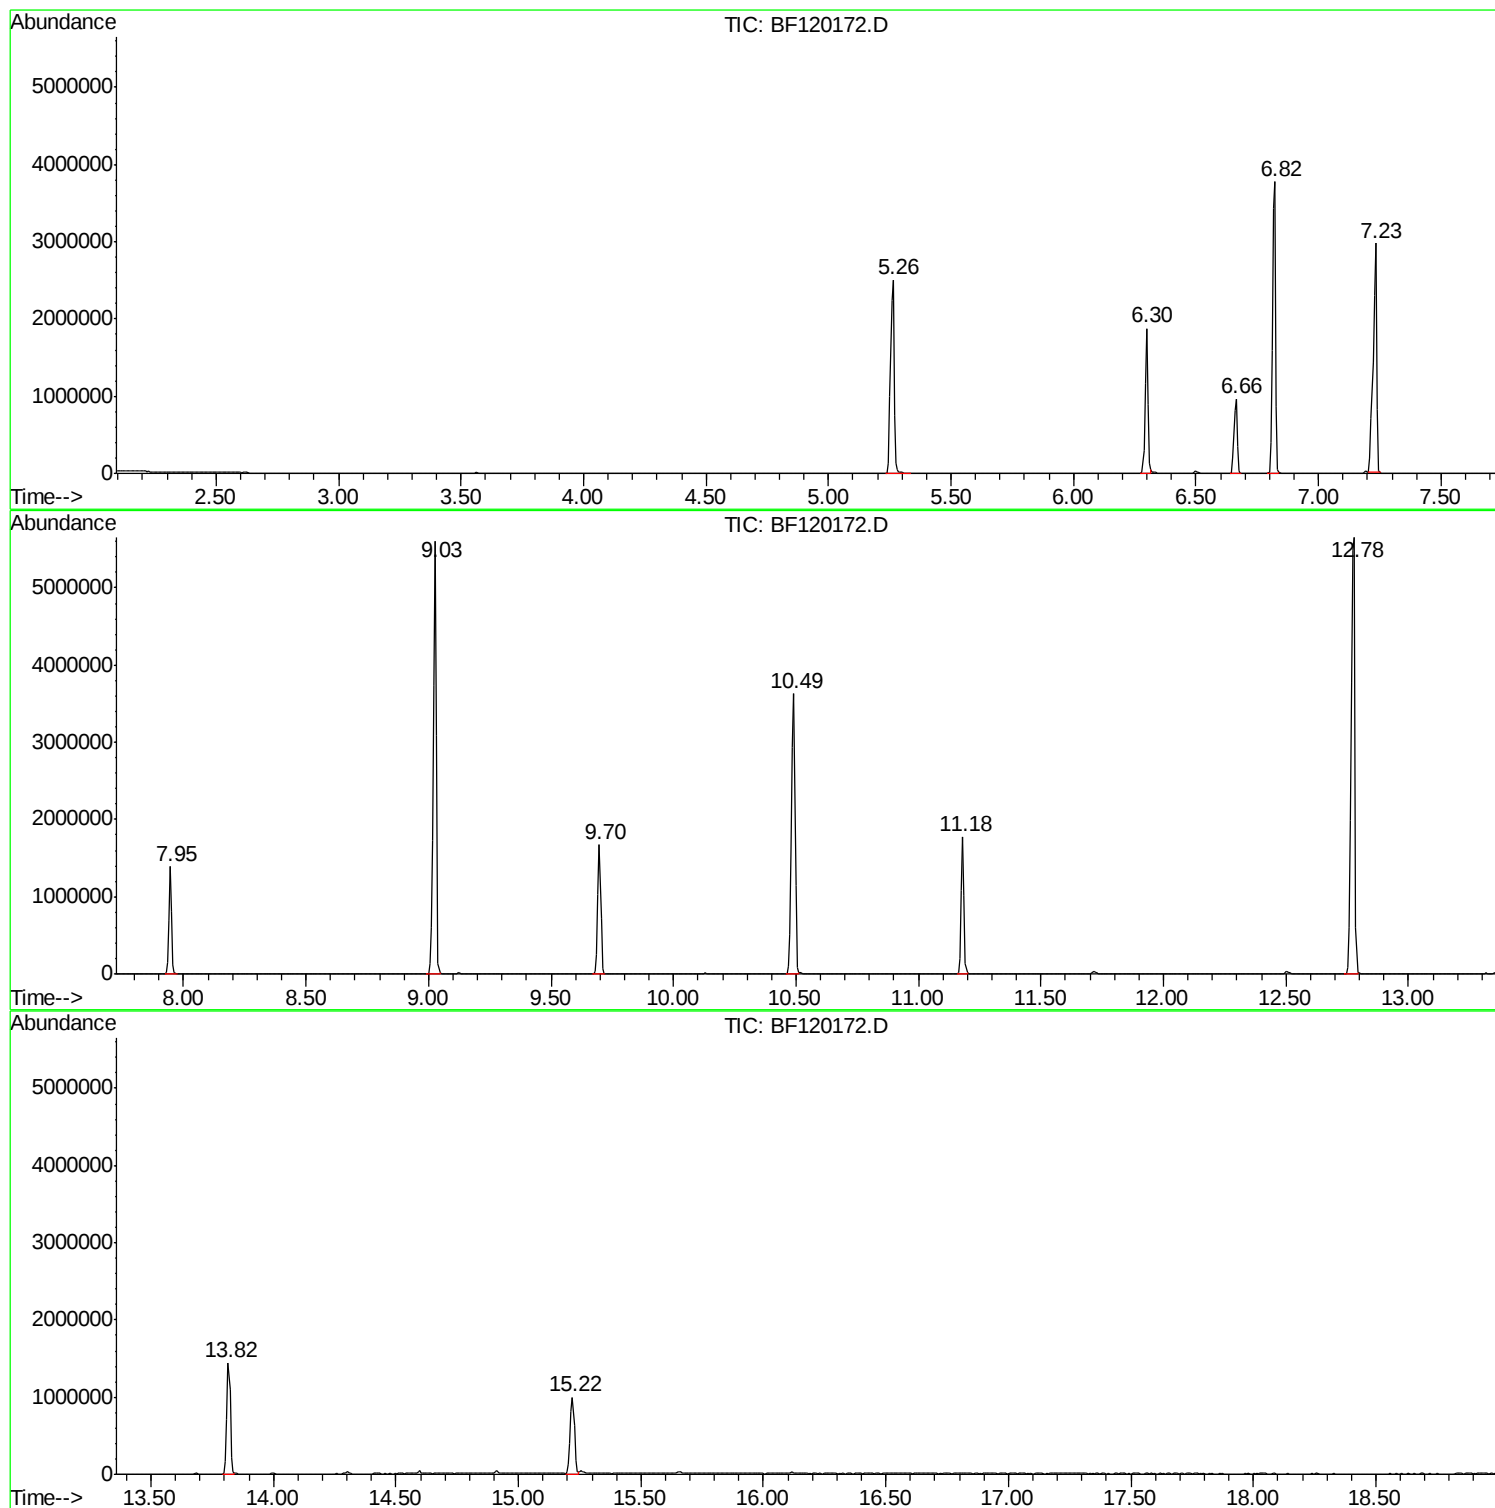

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120172.D
Acq On : 23 Apr 2020 19:12
Operator : MA/SJ
Sample : L2330-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120172.D
Acq On : 23 Apr 2020 19:12
Operator : MA/SJ
Sample : L2330-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PA-TWP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc