

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
 Data File : BF120173.D
 Acq On : 23 Apr 2020 19:39
 Operator : MA/SJ
 Sample : L2330-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-SO-2020-04-16

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	535	539	558	rBV	1965610	1896808	29.13%	5.757%
2	6.298	712	716	723	rBV	1316866	1113232	17.10%	3.379%
3	6.663	774	778	782	rBV	943836	842166	12.93%	2.556%
4	6.822	800	805	808	rBV	3820193	3584409	55.05%	10.879%
5	7.234	869	875	878	rBV	2929916	3012088	46.26%	9.142%
6	7.945	992	996	1000	rBV	1392820	1112543	17.09%	3.377%
7	9.027	1174	1180	1183	rBV	5884348	5525362	84.86%	16.770%
8	9.698	1290	1294	1297	rBV	1662565	1328701	20.41%	4.033%
9	10.492	1423	1429	1432	rBV	3841532	3726858	57.23%	11.311%
10	11.180	1542	1546	1550	rBV	1811650	1452860	22.31%	4.410%
11	12.780	1811	1818	1821	rBV	5840718	6511526	100.00%	19.763%
12	13.815	1990	1994	1998	rBV	1468792	1305400	20.05%	3.962%
13	14.598	2123	2127	2131	rVB	102105	92396	1.42%	0.280%
14	14.909	2175	2180	2184	rBV	104637	111578	1.71%	0.339%
15	15.221	2228	2233	2237	rBV	964946	1117820	17.17%	3.393%
16	15.257	2237	2239	2245	rVB	100410	112553	1.73%	0.342%
17	15.656	2301	2307	2316	rBV2	67968	101495	1.56%	0.308%


Sum of corrected areas: 32947795

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120173.D
Acq On : 23 Apr 2020 19:39
Operator : MA/SJ
Sample : L2330-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-SO-2020-04-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

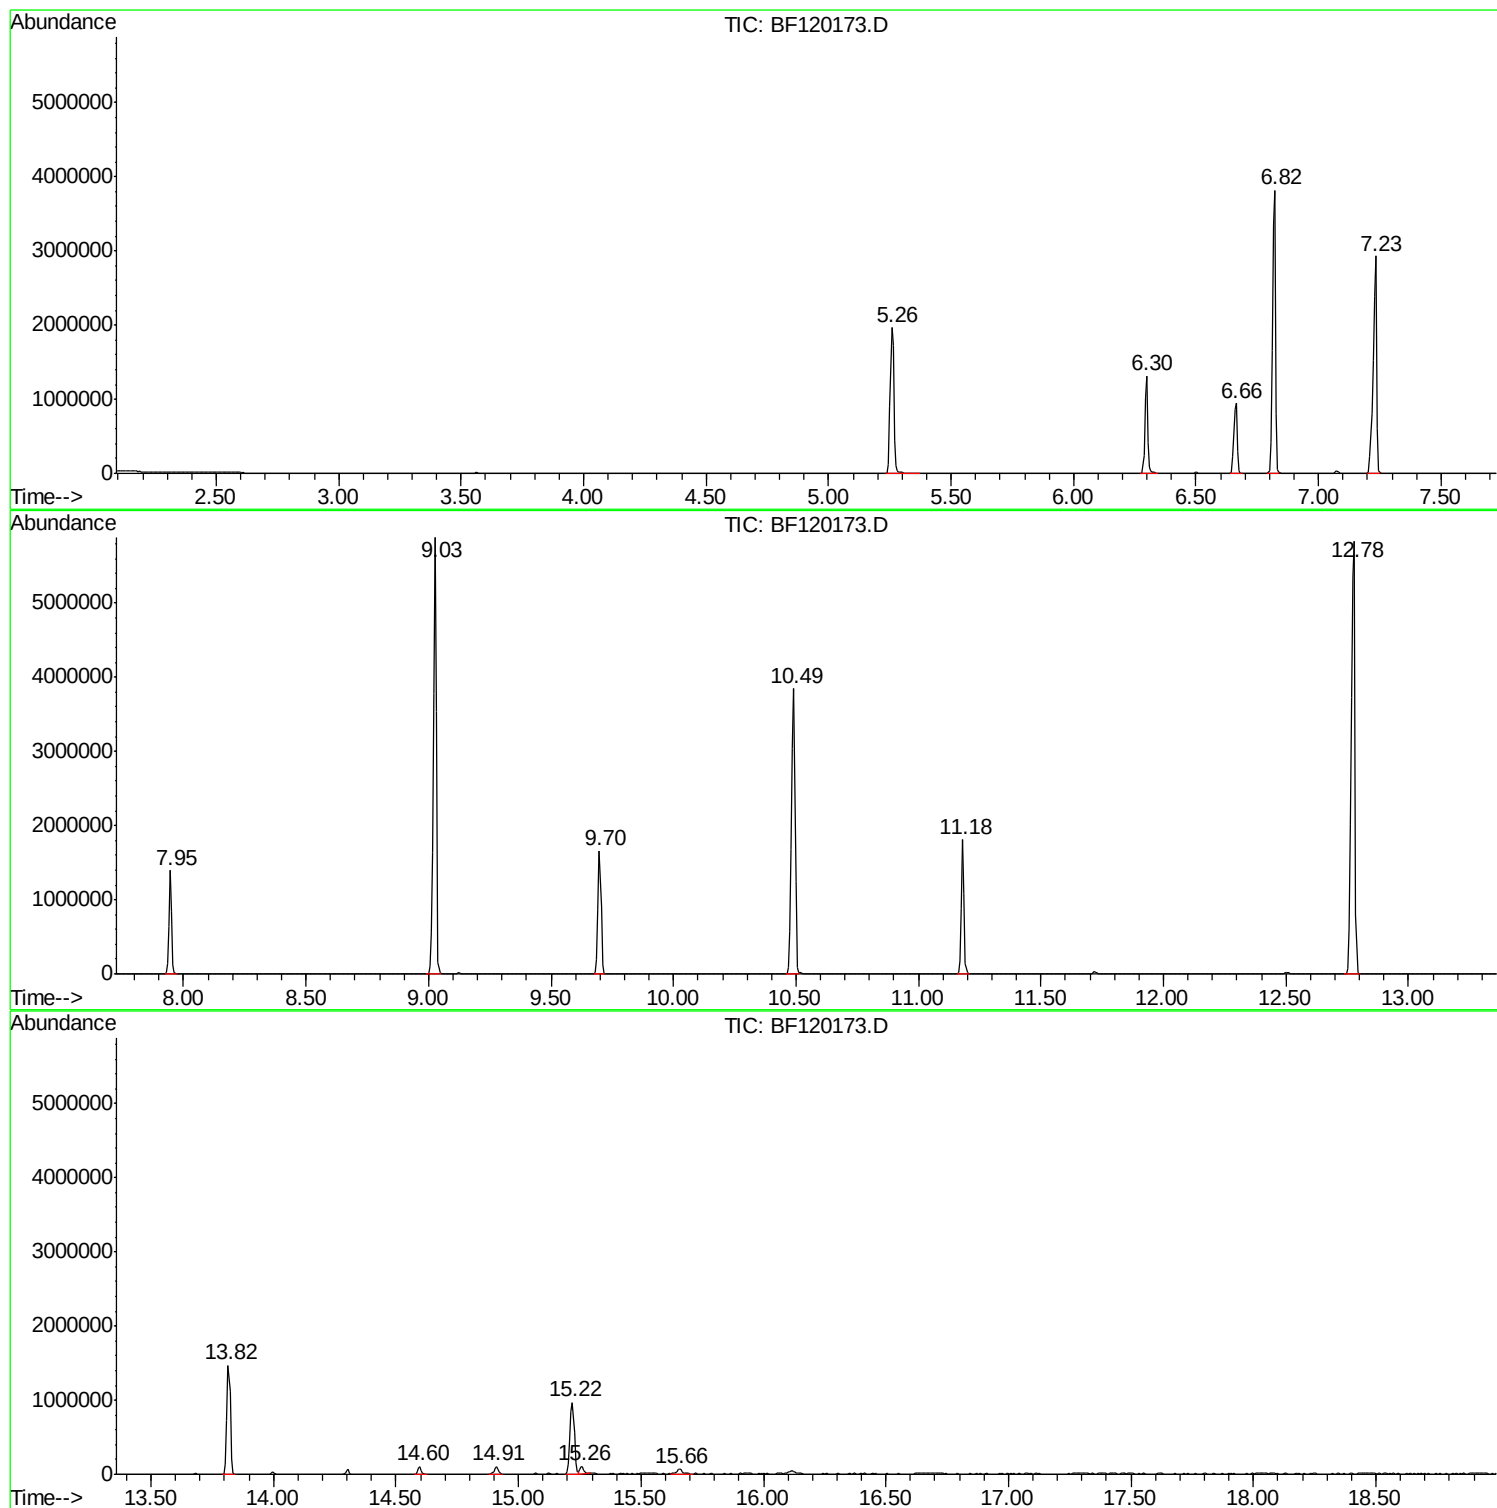

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120173.D
Acq On : 23 Apr 2020 19:39
Operator : MA/SJ
Sample : L2330-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-SO-2020-04-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
Data File : BF120173.D
Acq On : 23 Apr 2020 19:39
Operator : MA/SJ
Sample : L2330-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-SO-2020-04-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc