


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042320\  
 Data File : BF120157.D  
 Acq On : 23 Apr 2020 12:27  
 Operator : MA/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF040820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Apr 23 13:31:01 2020

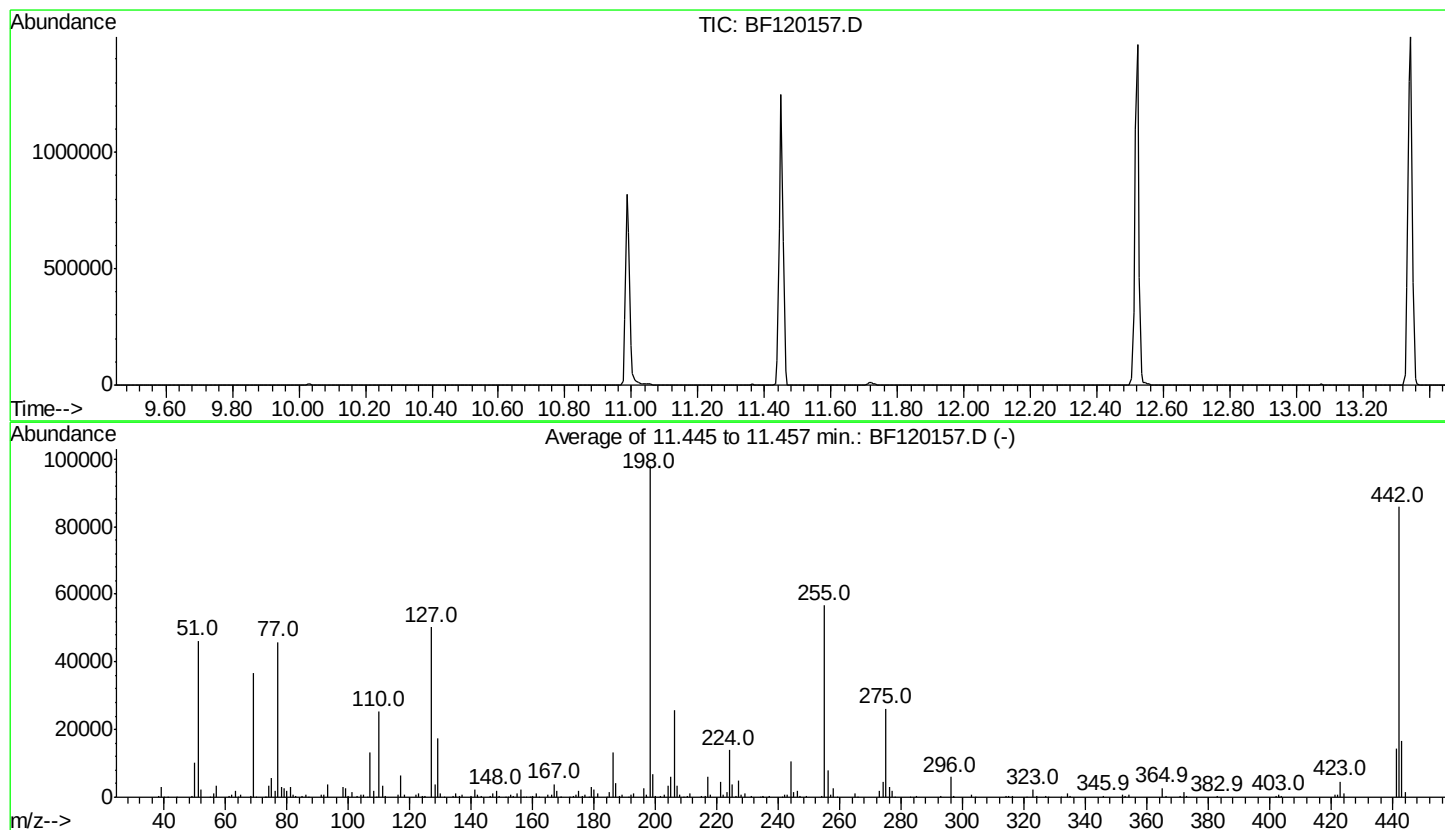

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 47.3      | 46346   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.2       | 449     | PASS             |
| 69          | 198          | 0.00         | 100          | 37.5      | 36802   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 172     | PASS             |
| 127         | 198          | 10           | 80           | 51.2      | 50229   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 652     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 98016   | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 6949    | PASS             |
| 275         | 198          | 10           | 60           | 26.7      | 26162   | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 2817    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.6      | 14355   | PASS             |
| 442         | 198          | 50           | 100          | 87.5      | 85786   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 16693   | PASS             |