


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042320\
 Data File : BF120181.D
 Acq On : 23 Apr 2020 23:16
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 13:31:01 2020

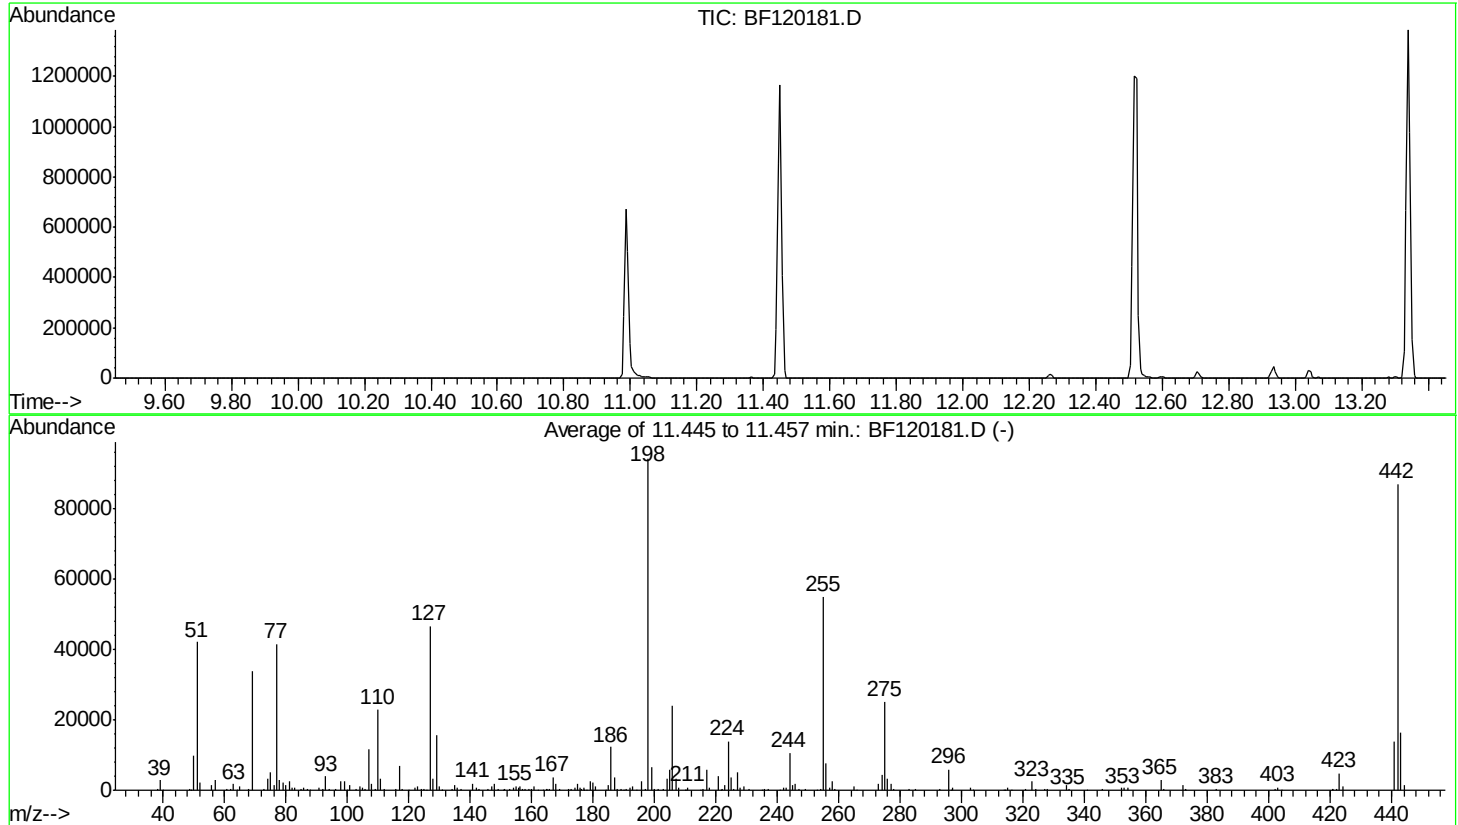

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	42115	PASS
68	69	0.00	2	1.5	520	PASS
69	198	0.00	100	35.7	33727	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	46770	PASS
197	198	0.00	2	0.6	544	PASS
198	198	100	100	100.0	94365	PASS
199	198	5	9	6.9	6474	PASS
275	198	10	60	26.7	25158	PASS
365	198	1	100	3.1	2949	PASS
441	198	0.01	100	14.7	13851	PASS
442	198	50	100	92.3	87088	PASS
443	442	15	24	19.0	16549	PASS