


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042420\
 Data File : BF120187.D
 Acq On : 24 Apr 2020 8:19
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 24 10:24:30 2020

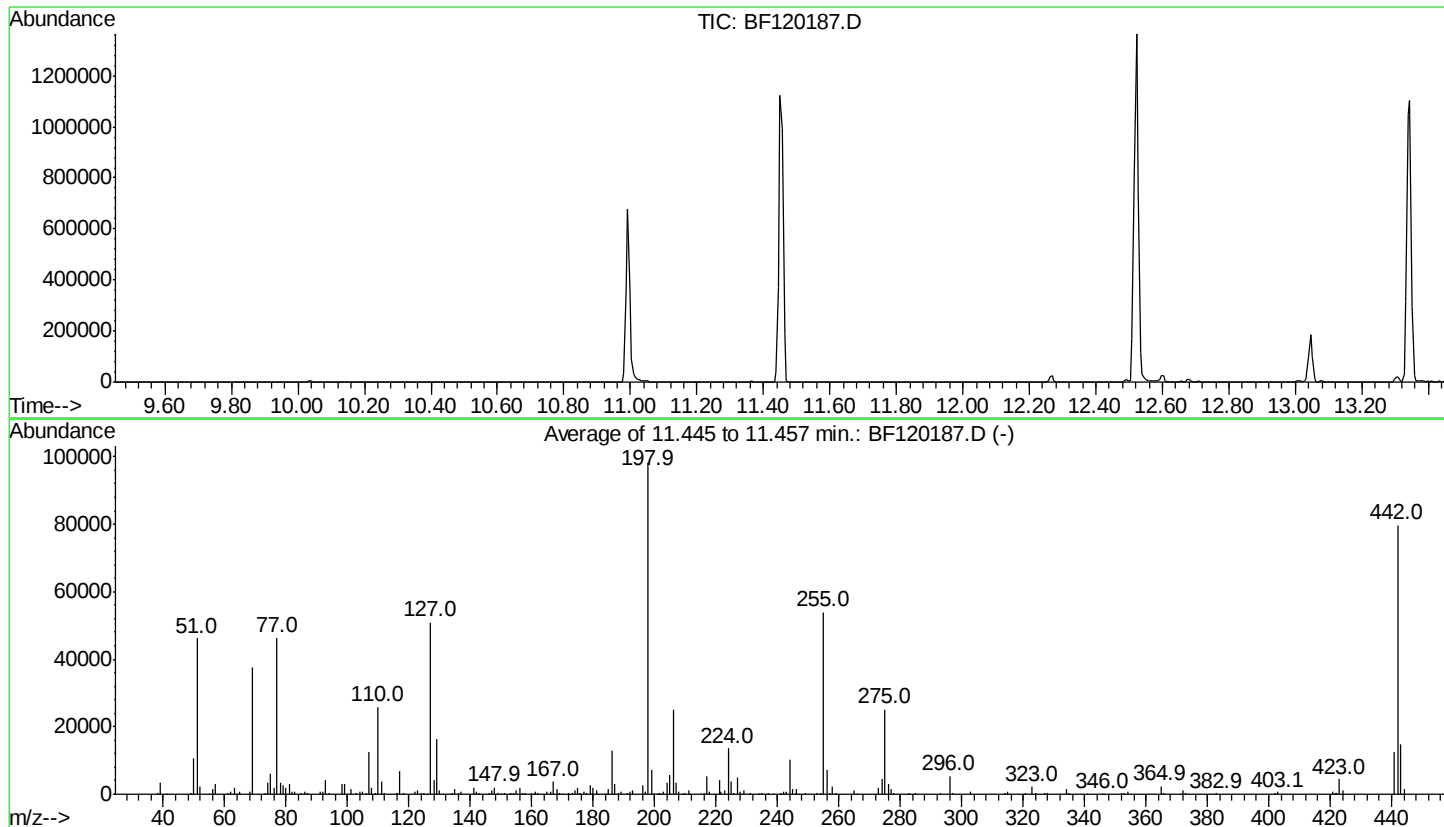

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	46248	PASS
68	69	0.00	2	1.8	689	PASS
69	198	0.00	100	38.4	37746	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	50968	PASS
197	198	0.00	2	0.6	610	PASS
198	198	100	100	100.0	98248	PASS
199	198	5	9	7.2	7041	PASS
275	198	10	60	25.5	25044	PASS
365	198	1	100	2.5	2430	PASS
441	198	0.01	100	12.8	12610	PASS
442	198	50	100	81.1	79727	PASS
443	442	15	24	18.5	14781	PASS