

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137718.D
Acq On : 24 Apr 2024 14:50
Operator : CG\JU
Sample : PB160476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160476BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.699	608	614	617	rBV	7024645	8124336	75.14%	13.172%
2	6.675	773	780	783	rBV	6745812	8090103	74.82%	13.117%
3	7.063	842	846	849	rBV	2134648	1756721	16.25%	2.848%
4	7.622	935	941	944	rBV	5085683	5314455	49.15%	8.617%
5	8.346	1059	1064	1067	rBV	2753790	2353990	21.77%	3.817%
6	9.422	1241	1247	1250	rBV	10041545	10056856	93.01%	16.306%
7	10.110	1358	1364	1367	rBV	2896750	2699064	24.96%	4.376%
8	10.898	1491	1498	1501	rBV	5905148	5919657	54.75%	9.598%
9	11.604	1614	1618	1621	rVB	3161375	2709261	25.06%	4.393%
10	13.198	1883	1889	1892	rBV	10361598	10812726	100.00%	17.531%
11	14.251	2064	2068	2072	rBV	2634989	2241244	20.73%	3.634%
12	15.827	2330	2336	2347	rBV	1270130	1598546	14.78%	2.592%




Sum of corrected areas: 61676959

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137718.D
Acq On : 24 Apr 2024 14:50
Operator : CG\JU
Sample : PB160476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160476BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

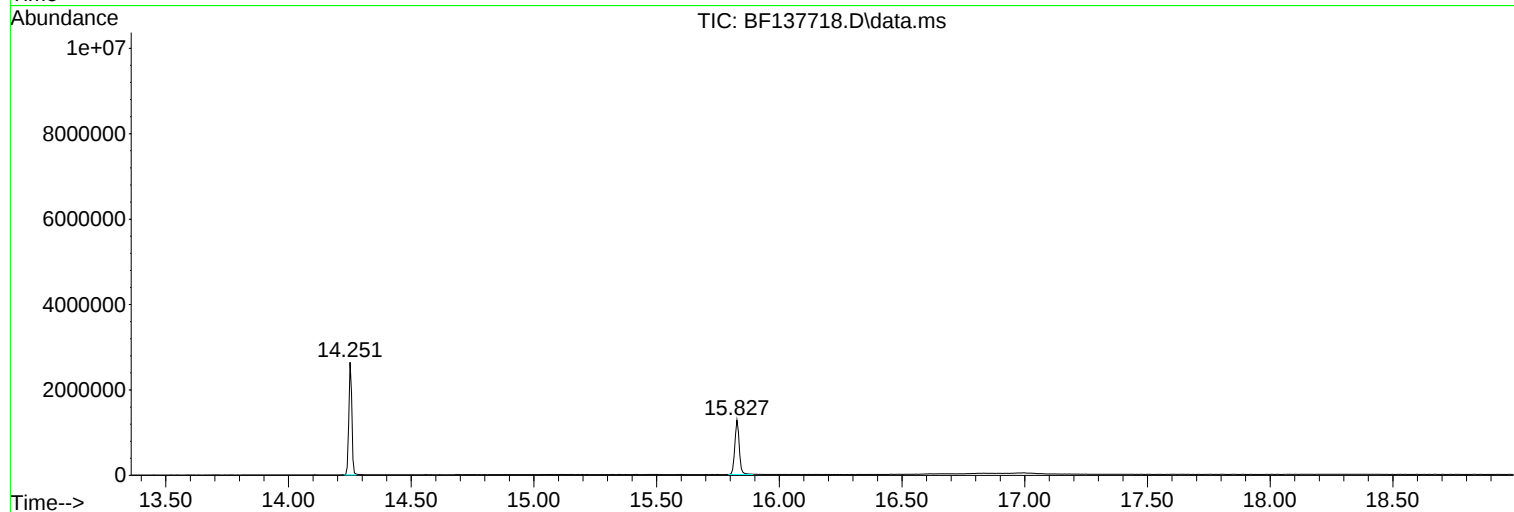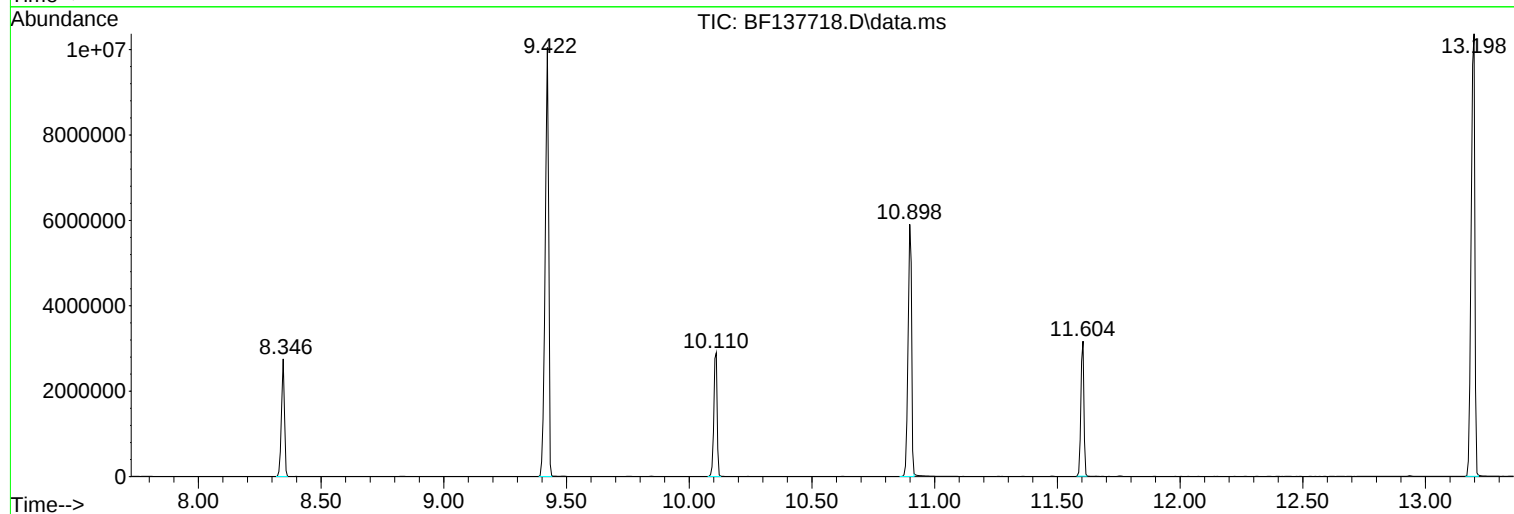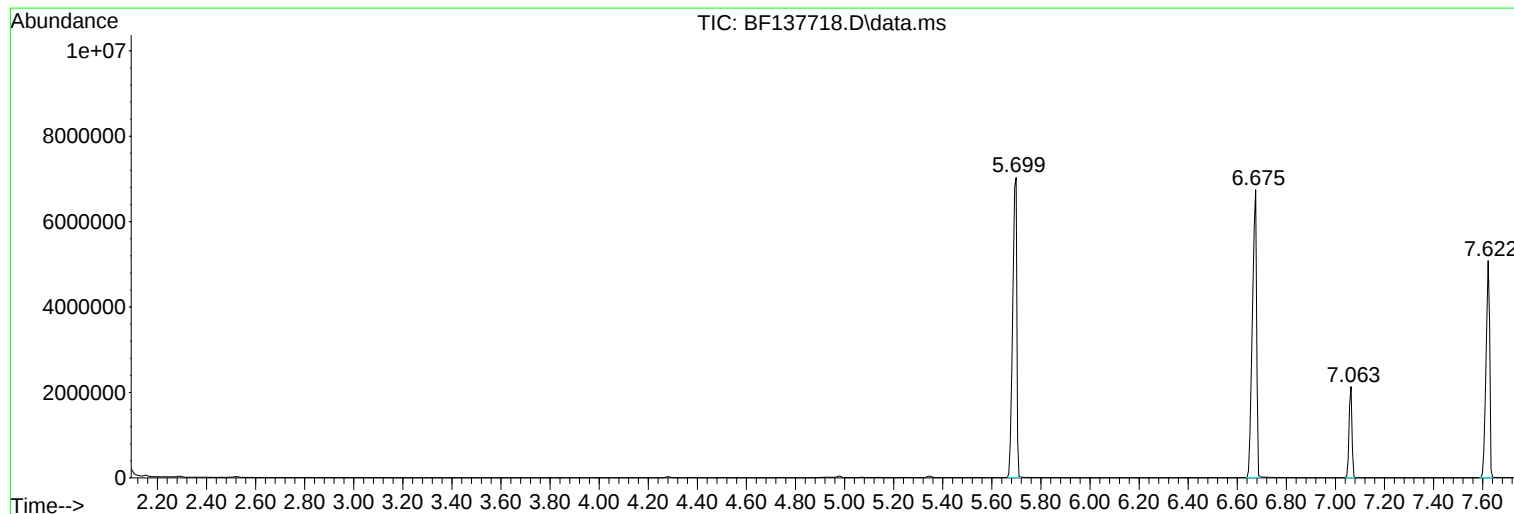

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137718.D
Acq On : 24 Apr 2024 14:50
Operator : CG\JU
Sample : PB160476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160476BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137718.D
Acq On : 24 Apr 2024 14:50
Operator : CG\JU
Sample : PB160476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160476BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------