


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137708.D
Acq On : 24 Apr 2024 09:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 24 03:57:12 2024

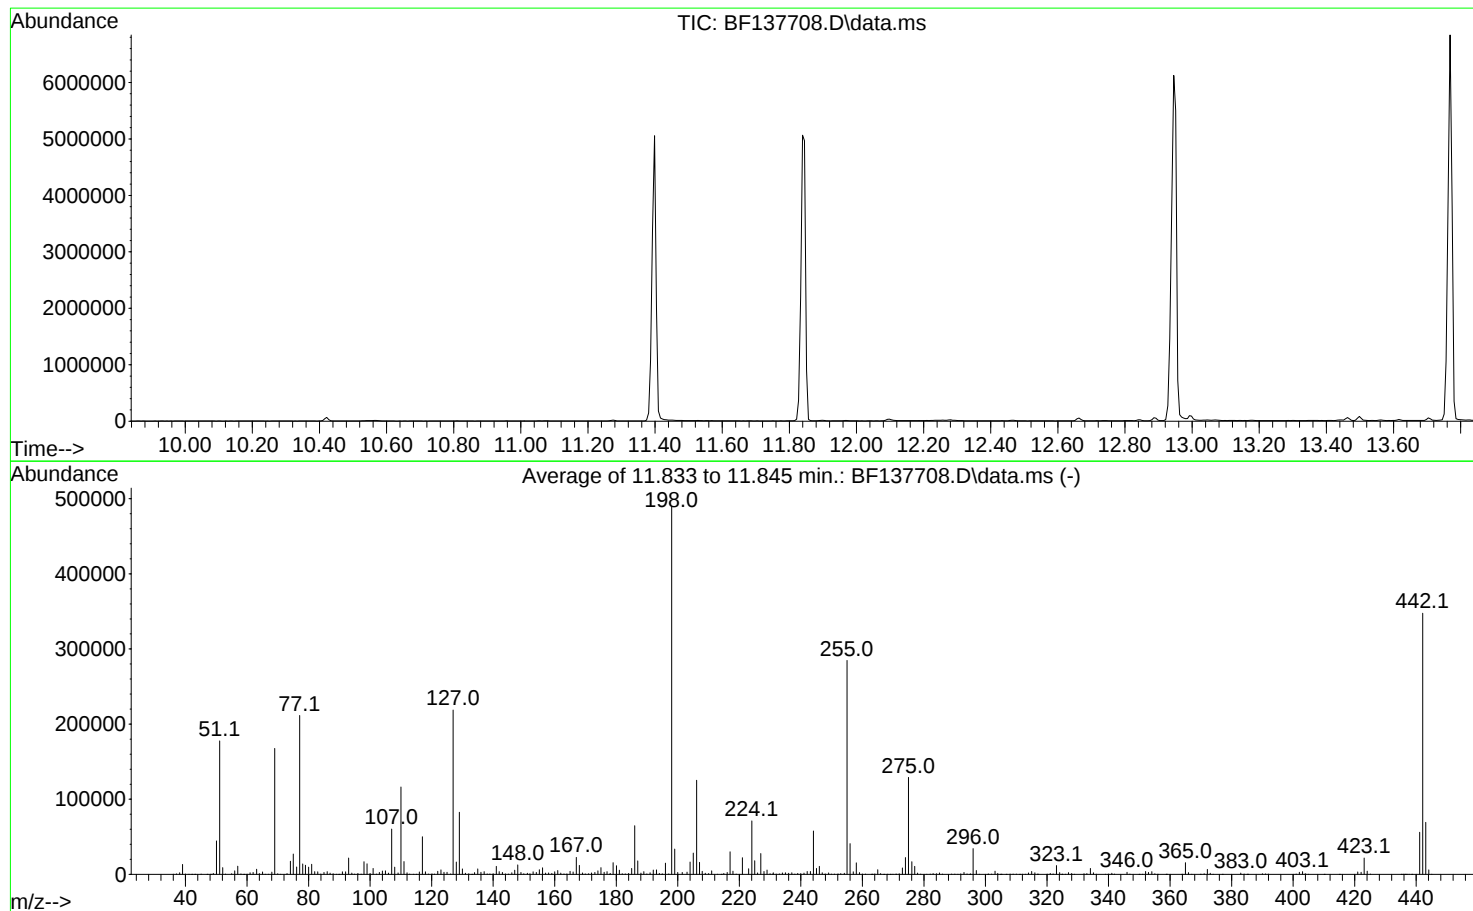




AutoFind: Scans 1657, 1658, 1659; Background Corrected with Scan 1651

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	177707	PASS
68	69	0.00	2	1.8	2933	PASS
69	198	0.00	100	34.2	167563	PASS
70	69	0.00	2	0.5	865	PASS
127	198	10	80	44.7	218688	PASS
197	198	0.00	2	0.1	547	PASS
198	198	100	100	100.0	489643	PASS
199	198	5	9	6.9	33619	PASS
275	198	10	60	26.4	129051	PASS
365	198	1	100	3.2	15645	PASS
441	198	0.01	100	11.5	56078	PASS
442	442	50	100	100.0	347536	PASS
443	442	15	24	19.9	69296	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137708.D
Acq On : 24 Apr 2024 09:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 24 13:59:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

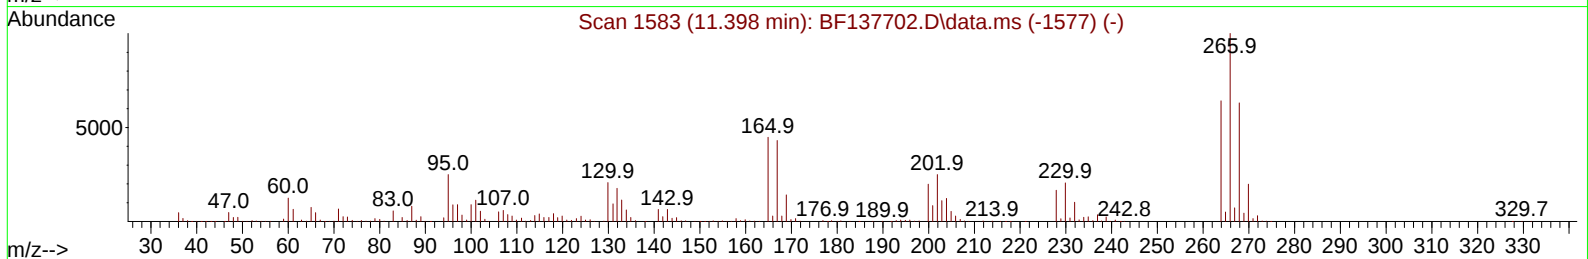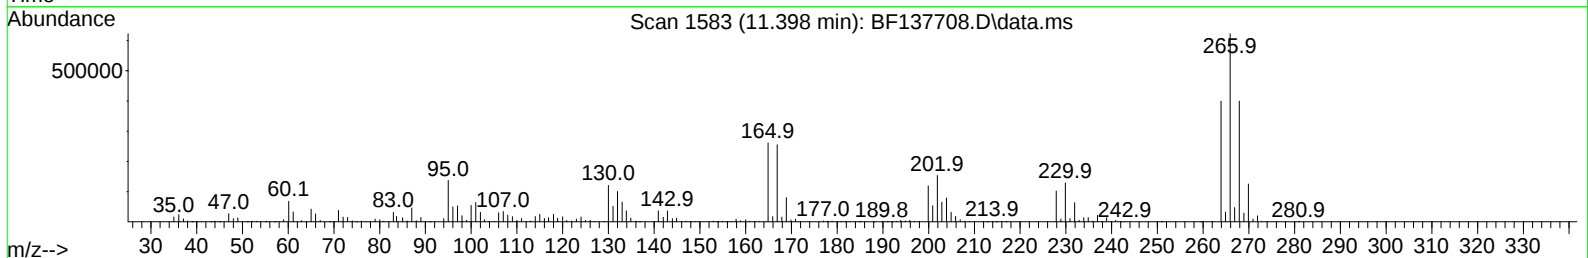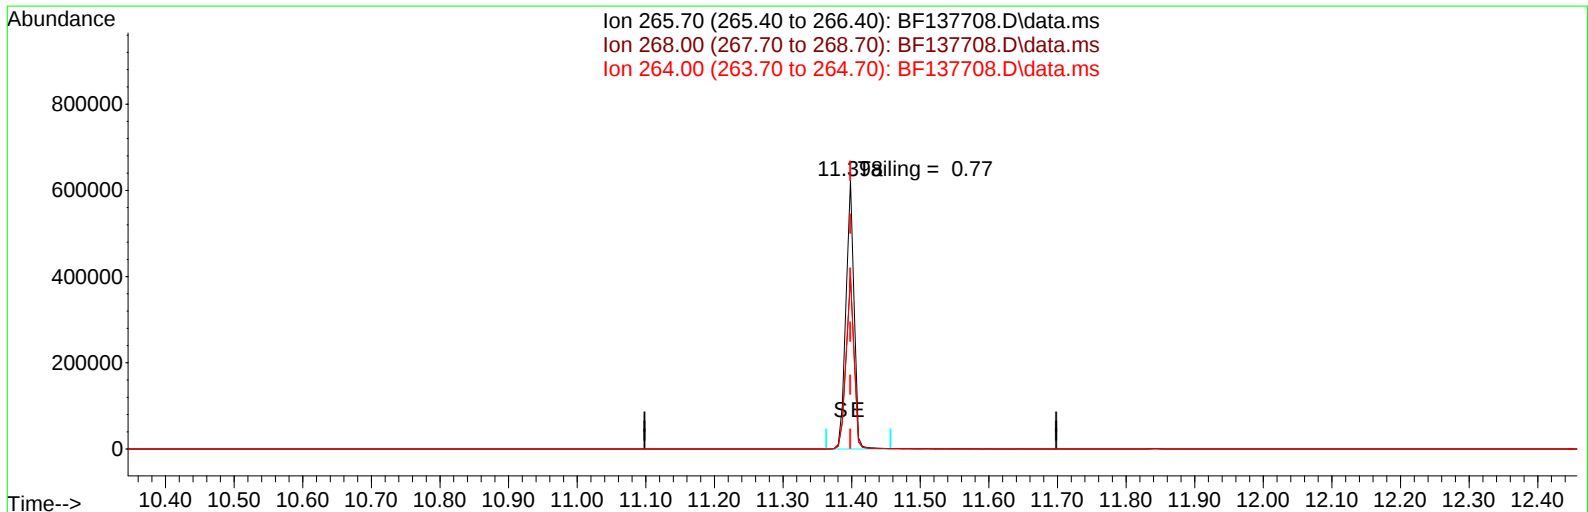

TIC: BF137708.D\data.ms

(70) Pentachlorophenol (C)

11.398min (+ 0.000) 304847.69 ng




response 512559

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.21
264.00	64.20	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042424\
Data File : BF137708.D
Acq On : 24 Apr 2024 09:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 24 13:59:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

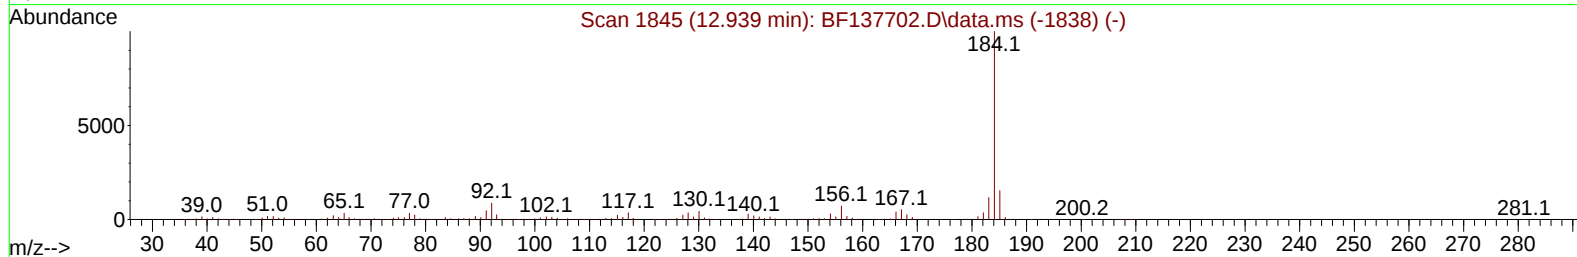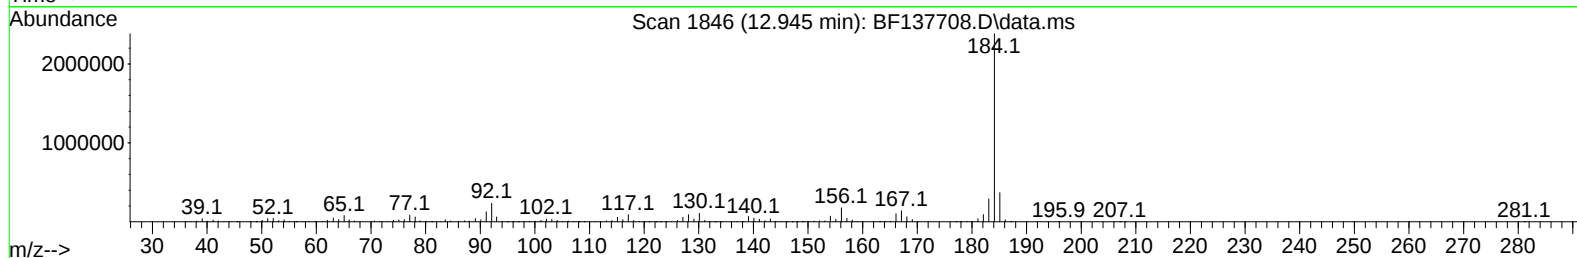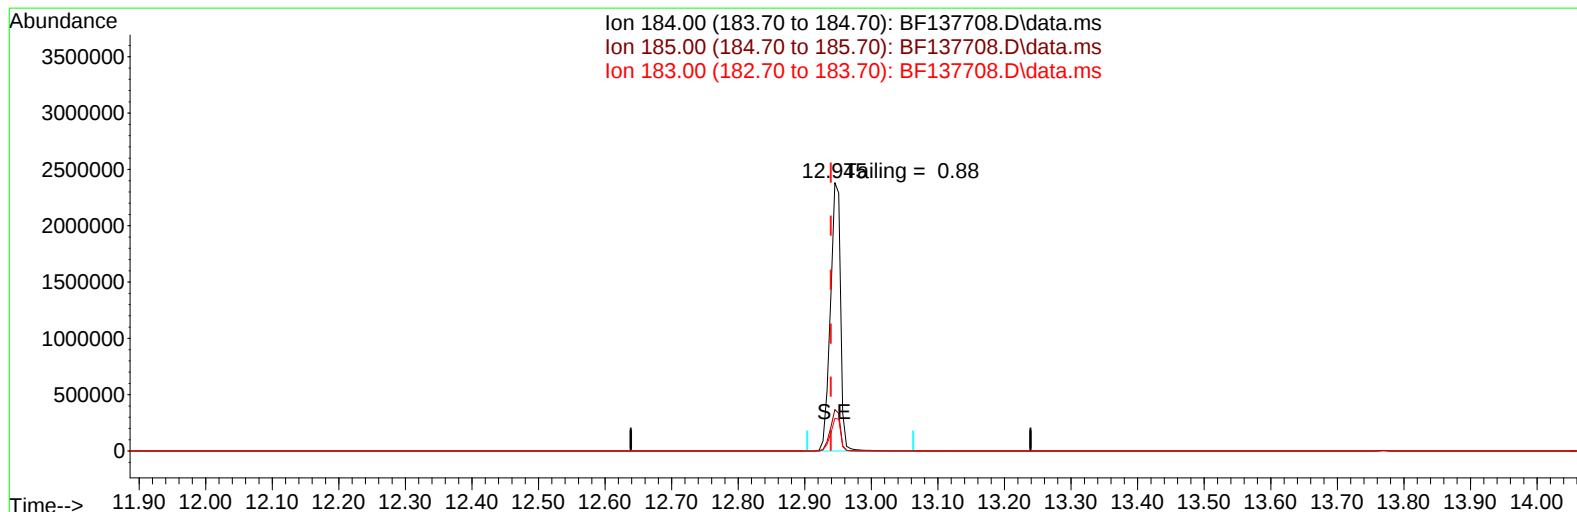

TIC: BF137708.D\data.ms

(77) Benzidine

12.945min (+ 0.006) 174639.08 ng

response 2537134

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.47
183.00	11.70	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/24/2024	BNA_F	<u>BF137708.D</u>
Compound Name	Response	Retention Time
DDT	1113756	13.769
DDD	16827	13.498
DDE	341	13.127
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17168	1130924	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP