
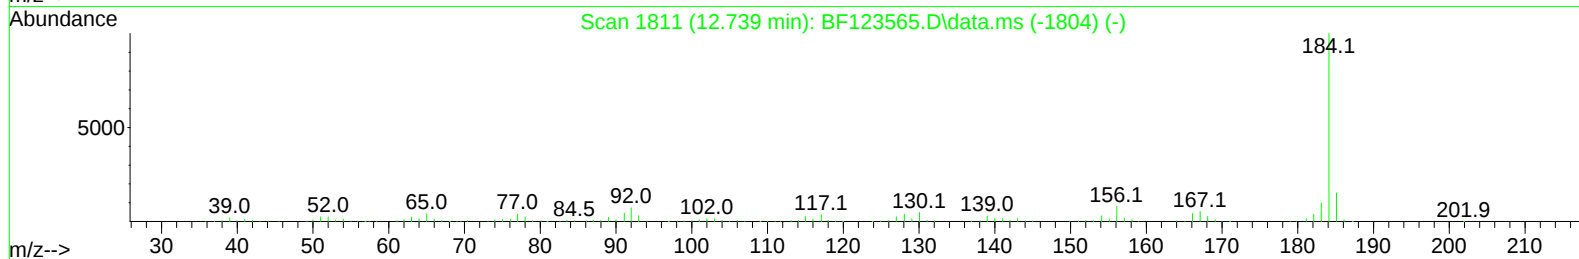
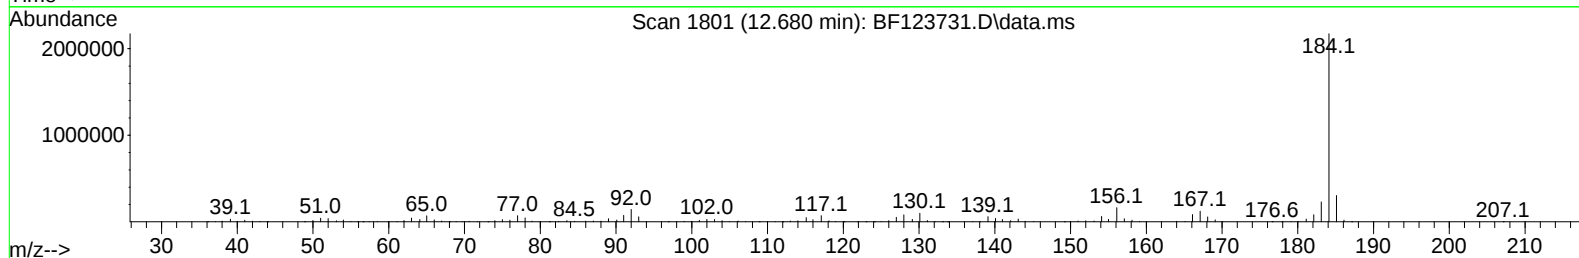


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042621\
Data File : BF123731.D
Acq On : 26 Apr 2021 14:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 14:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 14:53:39 2021
Response via : Initial Calibration

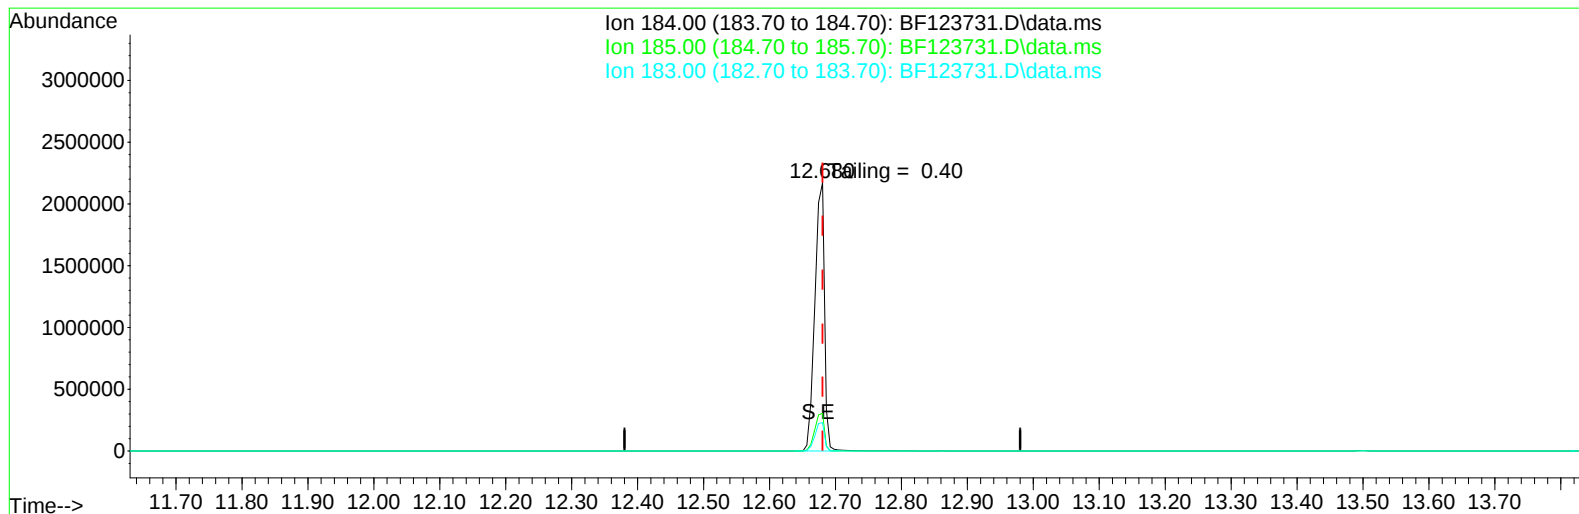

TIC: BF123731.D\data.ms

(77) Benzidine




12.680min (+ 0.000) 111175.19 ng

response 2200130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.00
183.00	9.80	10.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042621\
 Data File : BF123731.D
 Acq On : 26 Apr 2021 14:15
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 14:57:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 14:53:39 2021
 Response via : Initial Calibration

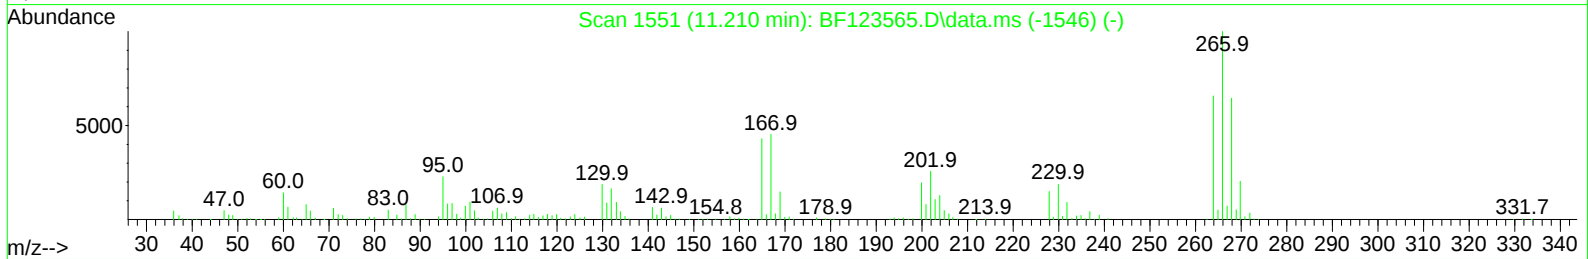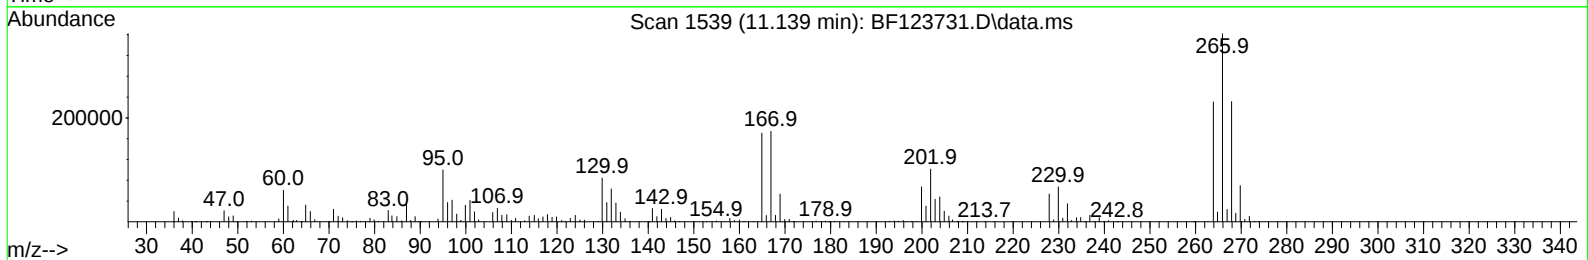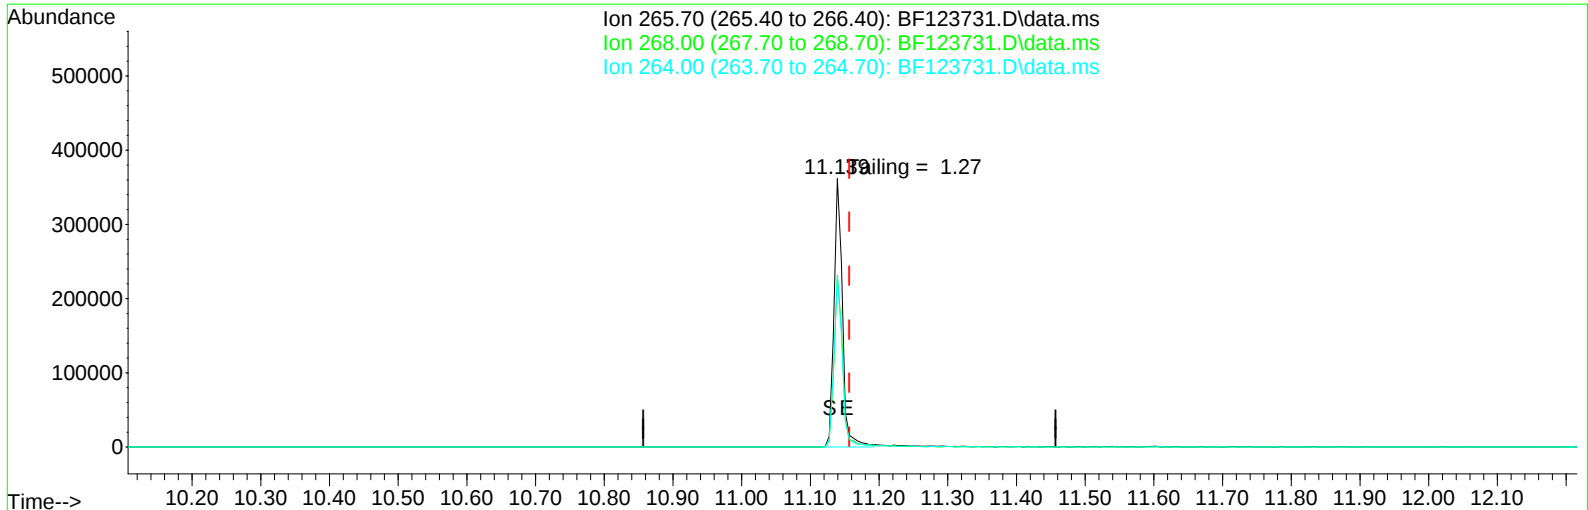

TIC: BF123731.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.018) 228774.33 ng

response 311238

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.96
264.00	65.70	63.78
0.00	0.00	0.00