


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042621\
 Data File : BF123731.D
 Acq On : 26 Apr 2021 14:15
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 19:04:46 2021

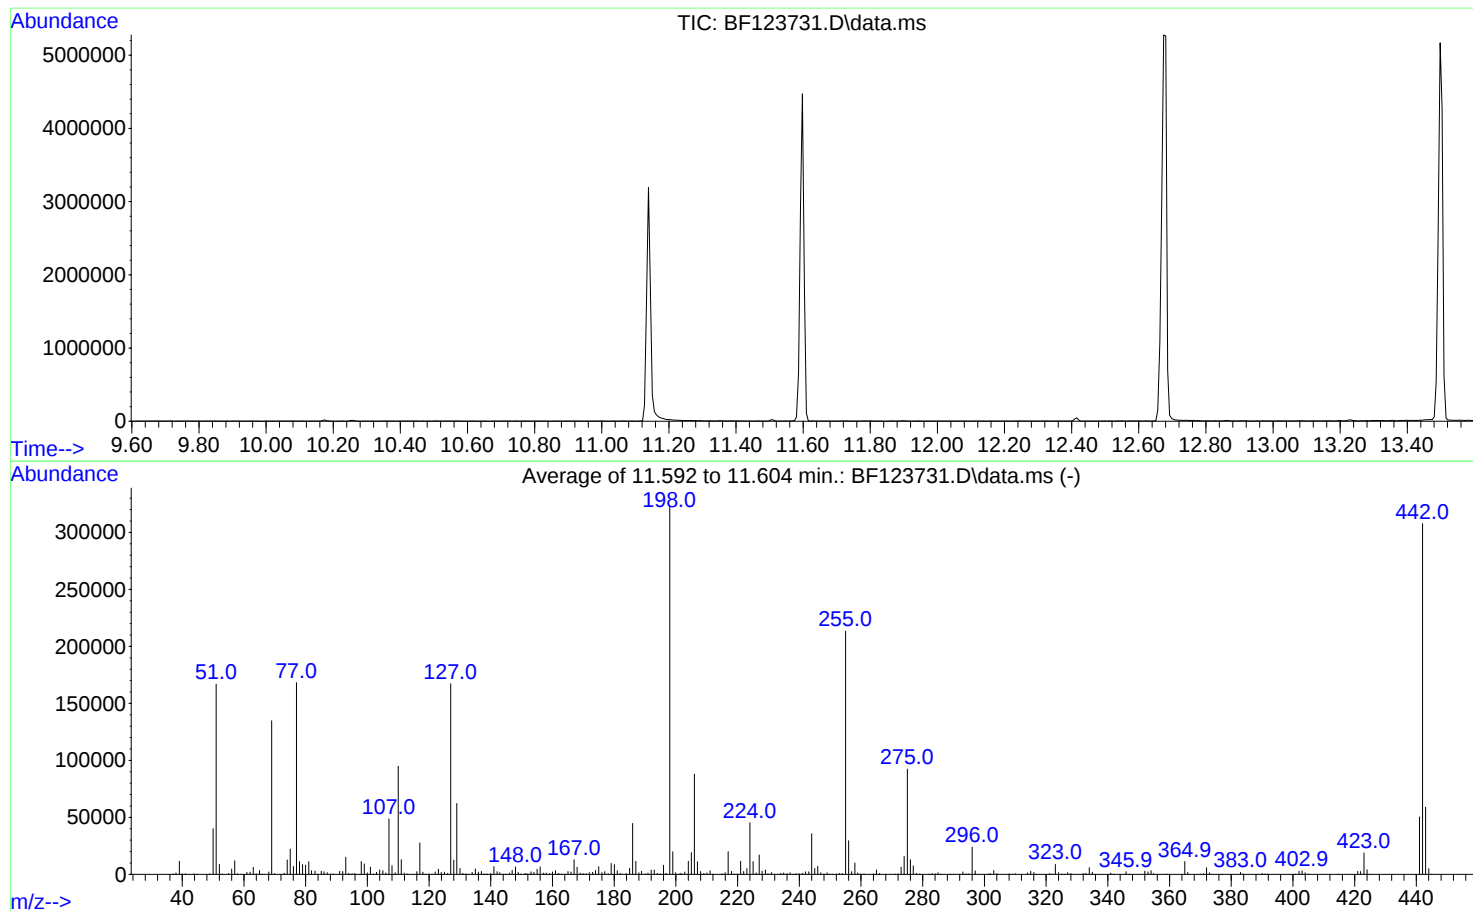




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	166989	PASS
68	69	0.00	2	1.5	2072	PASS
69	198	0.00	100	41.8	134789	PASS
70	69	0.00	2	0.5	714	PASS
127	198	10	80	51.8	167203	PASS
197	198	0.00	2	0.3	1009	PASS
198	198	100	100	100.0	322731	PASS
199	198	5	9	6.1	19771	PASS
275	198	10	60	28.6	92395	PASS
365	198	1	100	3.5	11242	PASS
441	198	0.01	100	15.6	50381	PASS
442	442	50	100	100.0	307669	PASS
443	442	15	24	19.2	59037	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042621\
Data File : BF123731.D
Acq On : 26 Apr 2021 14:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 14:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 14:53:39 2021
Response via : Initial Calibration

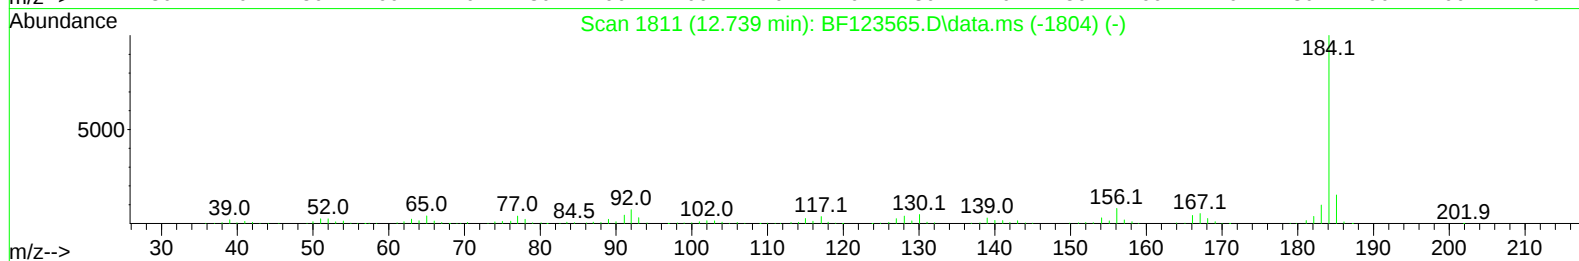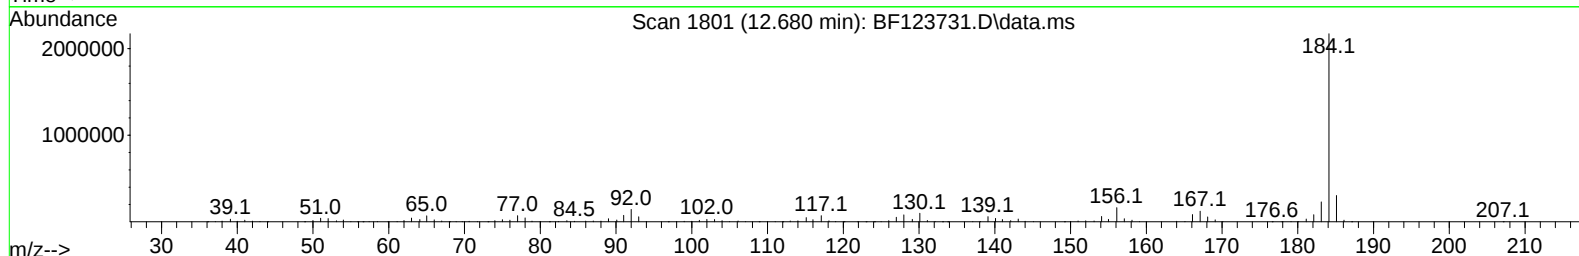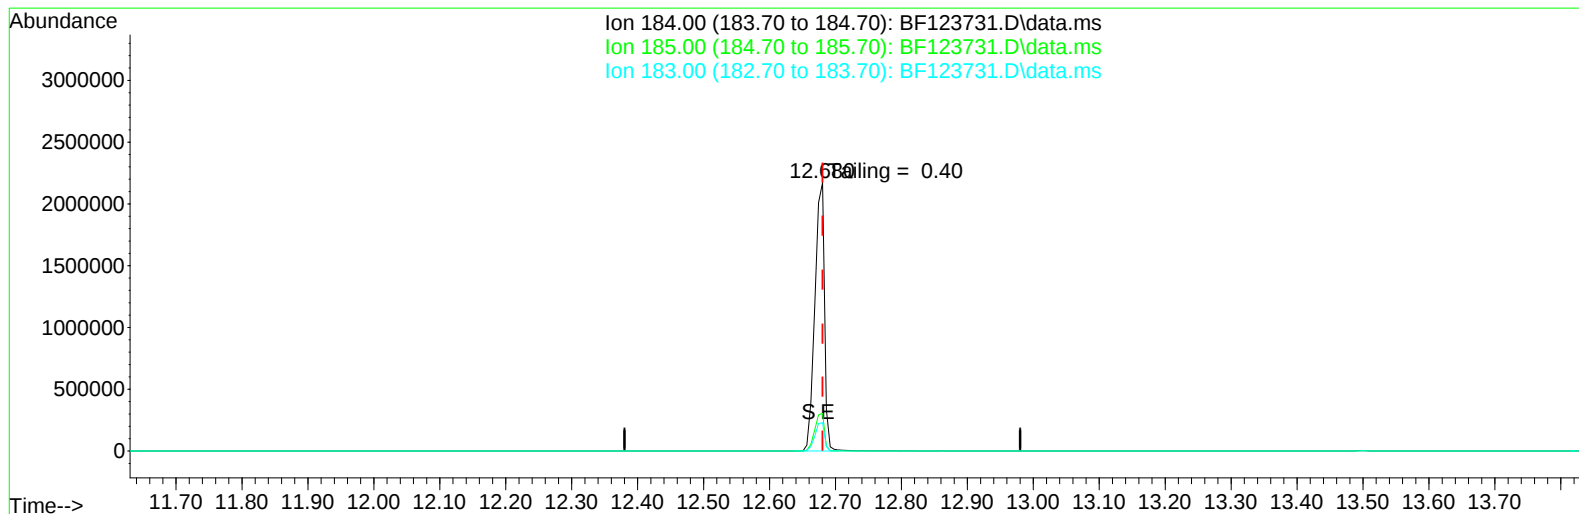

TIC: BF123731.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 111175.19 ng




response 2200130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.00
183.00	9.80	10.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042621\
 Data File : BF123731.D
 Acq On : 26 Apr 2021 14:15
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 26 14:57:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 14:53:39 2021
 Response via : Initial Calibration

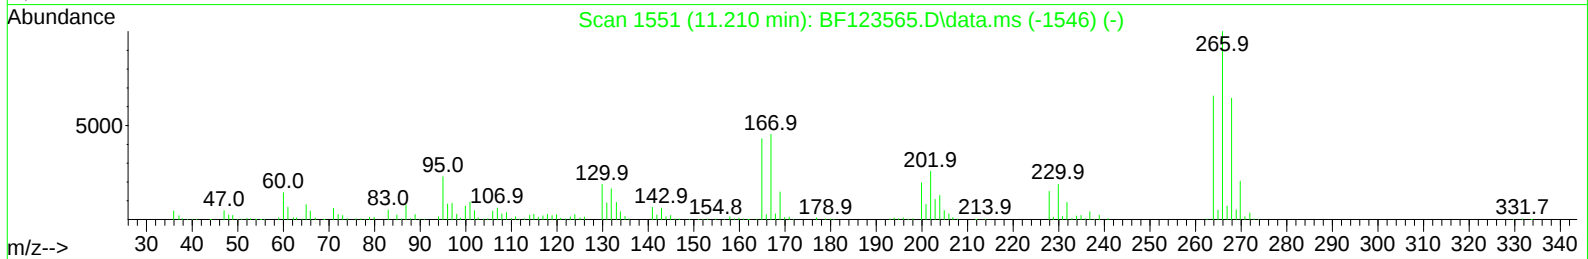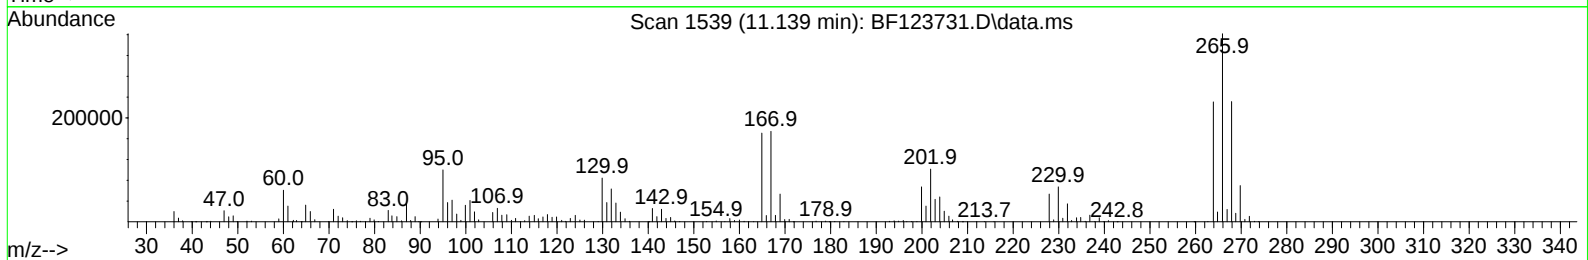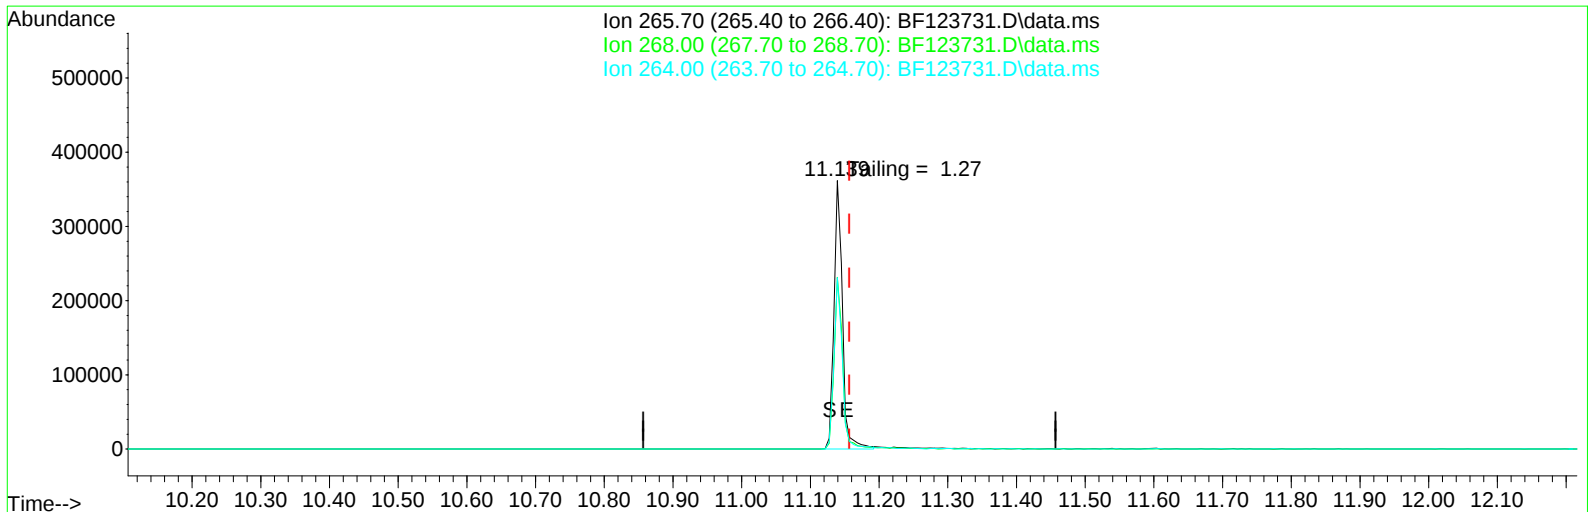

TIC: BF123731.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.018) 228774.33 ng

response 311238

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.96
264.00	65.70	63.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2021	BNA_F	<u>BF123731.D</u>
Compound Name	Response	Retention Time
DDT	876848	13.49
DDD	3552	13.23
DDE	1032	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4584	881432	0.52