


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042624\
Data File : BF137729.D
Acq On : 26 Apr 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 24 03:57:12 2024

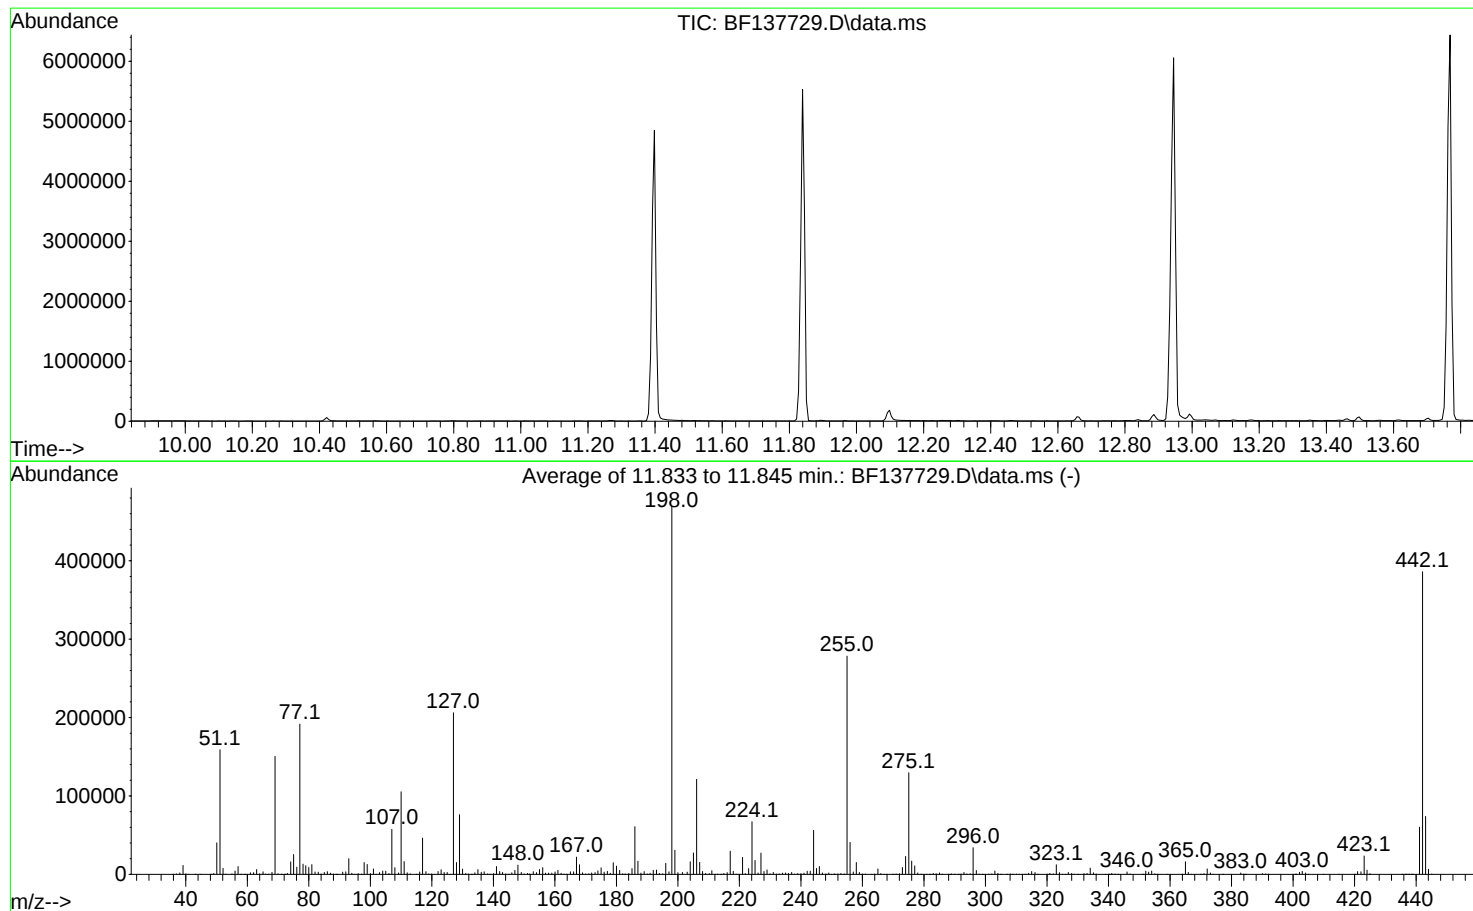

AutoFind: Scans 1657, 1658, 1659; Background Corrected with Scan 1651

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	33.9	158955	PASS
68	69	0.00	2	1.8	2645	PASS
69	198	0.00	100	32.1	150521	PASS
70	69	0.00	2	0.6	842	PASS
127	198	10	80	43.9	206144	PASS
197	198	0.00	2	0.7	3243	PASS
198	198	100	100	100.0	469163	PASS
199	198	5	9	6.6	30899	PASS
275	198	10	60	27.6	129523	PASS
365	198	1	100	3.4	16110	PASS
441	198	0.01	100	12.8	60235	PASS
442	442	50	100	100.0	385899	PASS
443	442	15	24	19.1	73837	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/26/2024	BNA_F	<u>BF137729.D</u>
Compound Name	Response	Retention Time
DDT	1071837	13.768
DDD	13901	13.498
DDE	1502	13.127
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15403	1087240	1.42

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042624\
Data File : BF137729.D
Acq On : 26 Apr 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 18:37:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

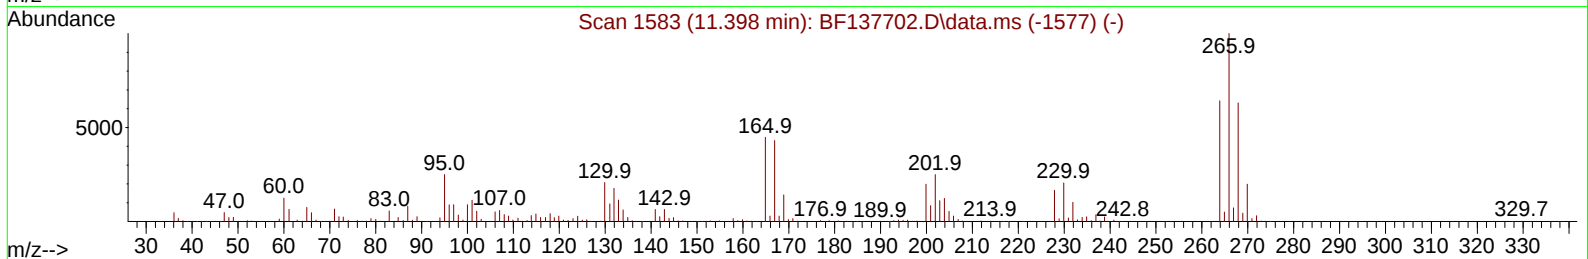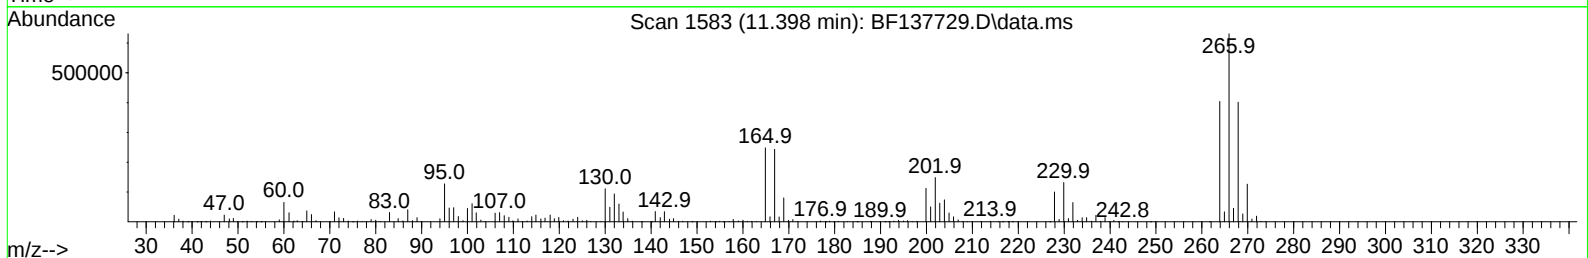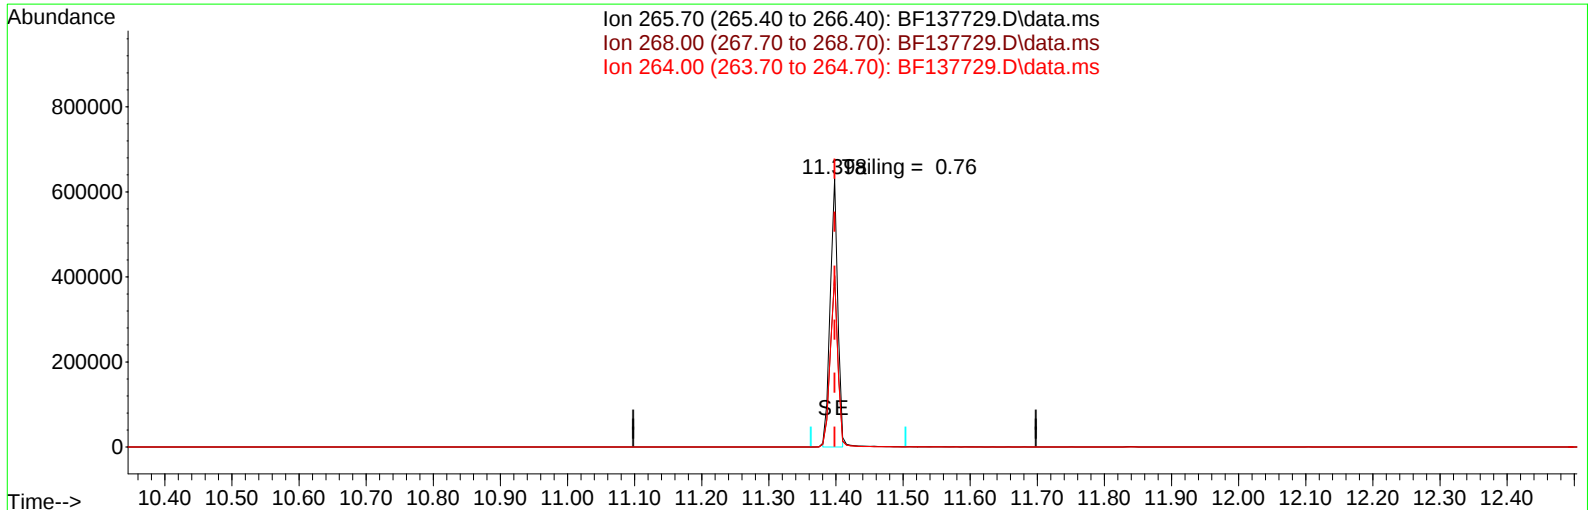

TIC: BF137729.D\data.ms

(70) Pentachlorophenol (C)

11.398min (0.000) 184894.28 ng




response 510273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.59
264.00	64.20	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042624\
Data File : BF137729.D
Acq On : 26 Apr 2024 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 18:37:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

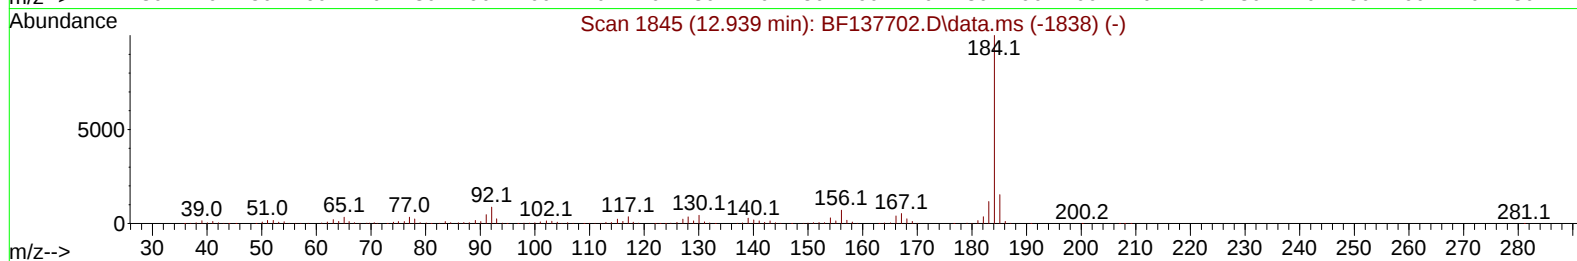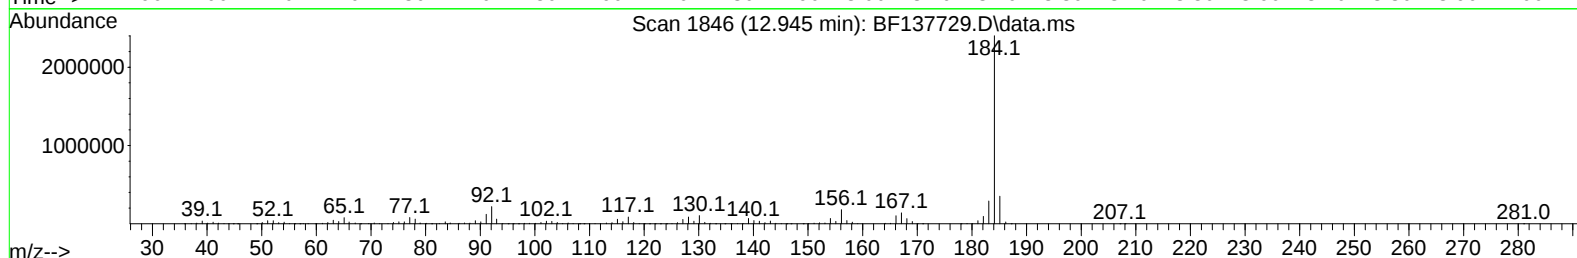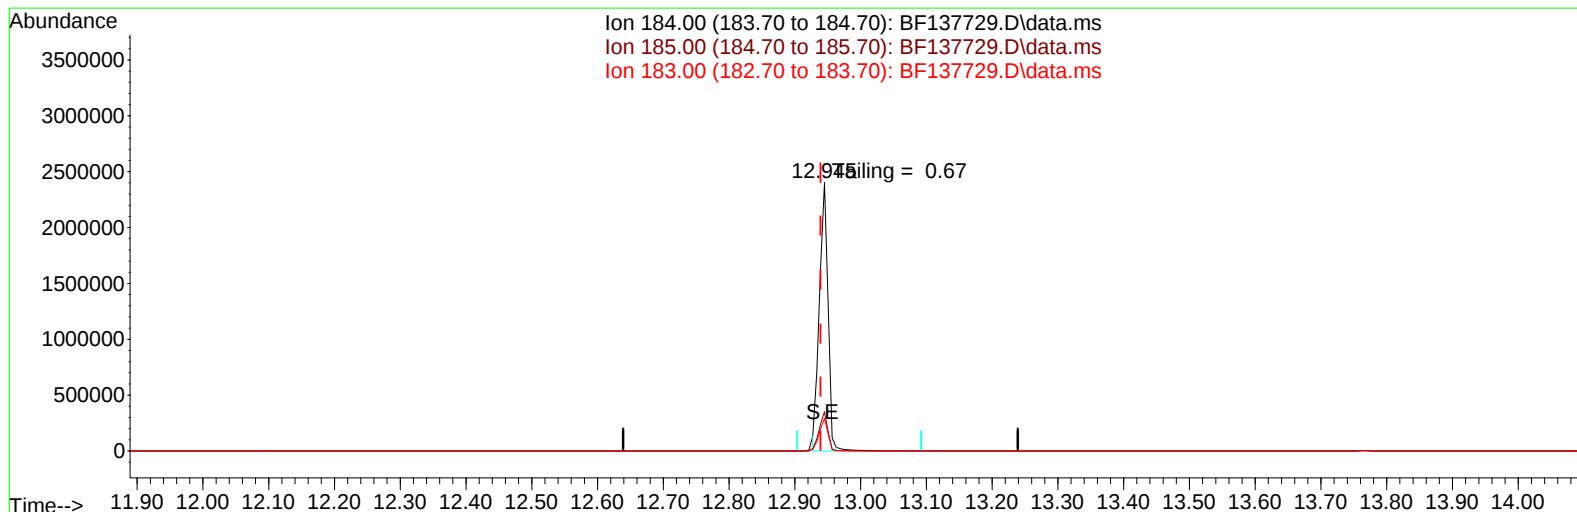

TIC: BF137729.D\data.ms

(77) Benzidine

12.945min (+ 0.006) 55807.14 ng

response 2271950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.61
183.00	11.70	12.12
0.00	0.00	0.00