

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042720\
Data File : BF120216.D
Acq On : 27 Apr 2020 14:01
Operator : MA/SJ
Sample : PB128487BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128487BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.275	538	542	559	rBV	3932851	4012781	77.42%	12.343%
2	6.316	714	719	722	rBV	3528258	3939762	76.02%	12.119%
3	6.663	774	778	787	rVB	893099	732014	14.12%	2.252%
4	6.822	800	805	808	rBV	3635616	3268534	63.07%	10.054%
5	7.233	869	875	878	rBV	2638384	2636507	50.87%	8.110%
6	7.945	992	996	1000	rBV	1017907	928439	17.91%	2.856%
7	9.027	1175	1180	1183	rBV	4677359	4812941	92.86%	14.804%
8	9.704	1290	1295	1298	rBV	1174111	1067577	20.60%	3.284%
9	10.498	1424	1430	1433	rBV	3000758	3052948	58.91%	9.391%
10	11.186	1543	1547	1550	rBV	1383528	1121064	21.63%	3.448%
11	12.780	1812	1818	1821	rBV	5124914	5182798	100.00%	15.942%
12	13.821	1991	1995	1999	rBV	1008408	959728	18.52%	2.952%
13	15.233	2230	2235	2239	rBV	672967	795187	15.34%	2.446%


Sum of corrected areas: 32510280

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042720\
Data File : BF120216.D
Acq On : 27 Apr 2020 14:01
Operator : MA/SJ
Sample : PB128487BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128487BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

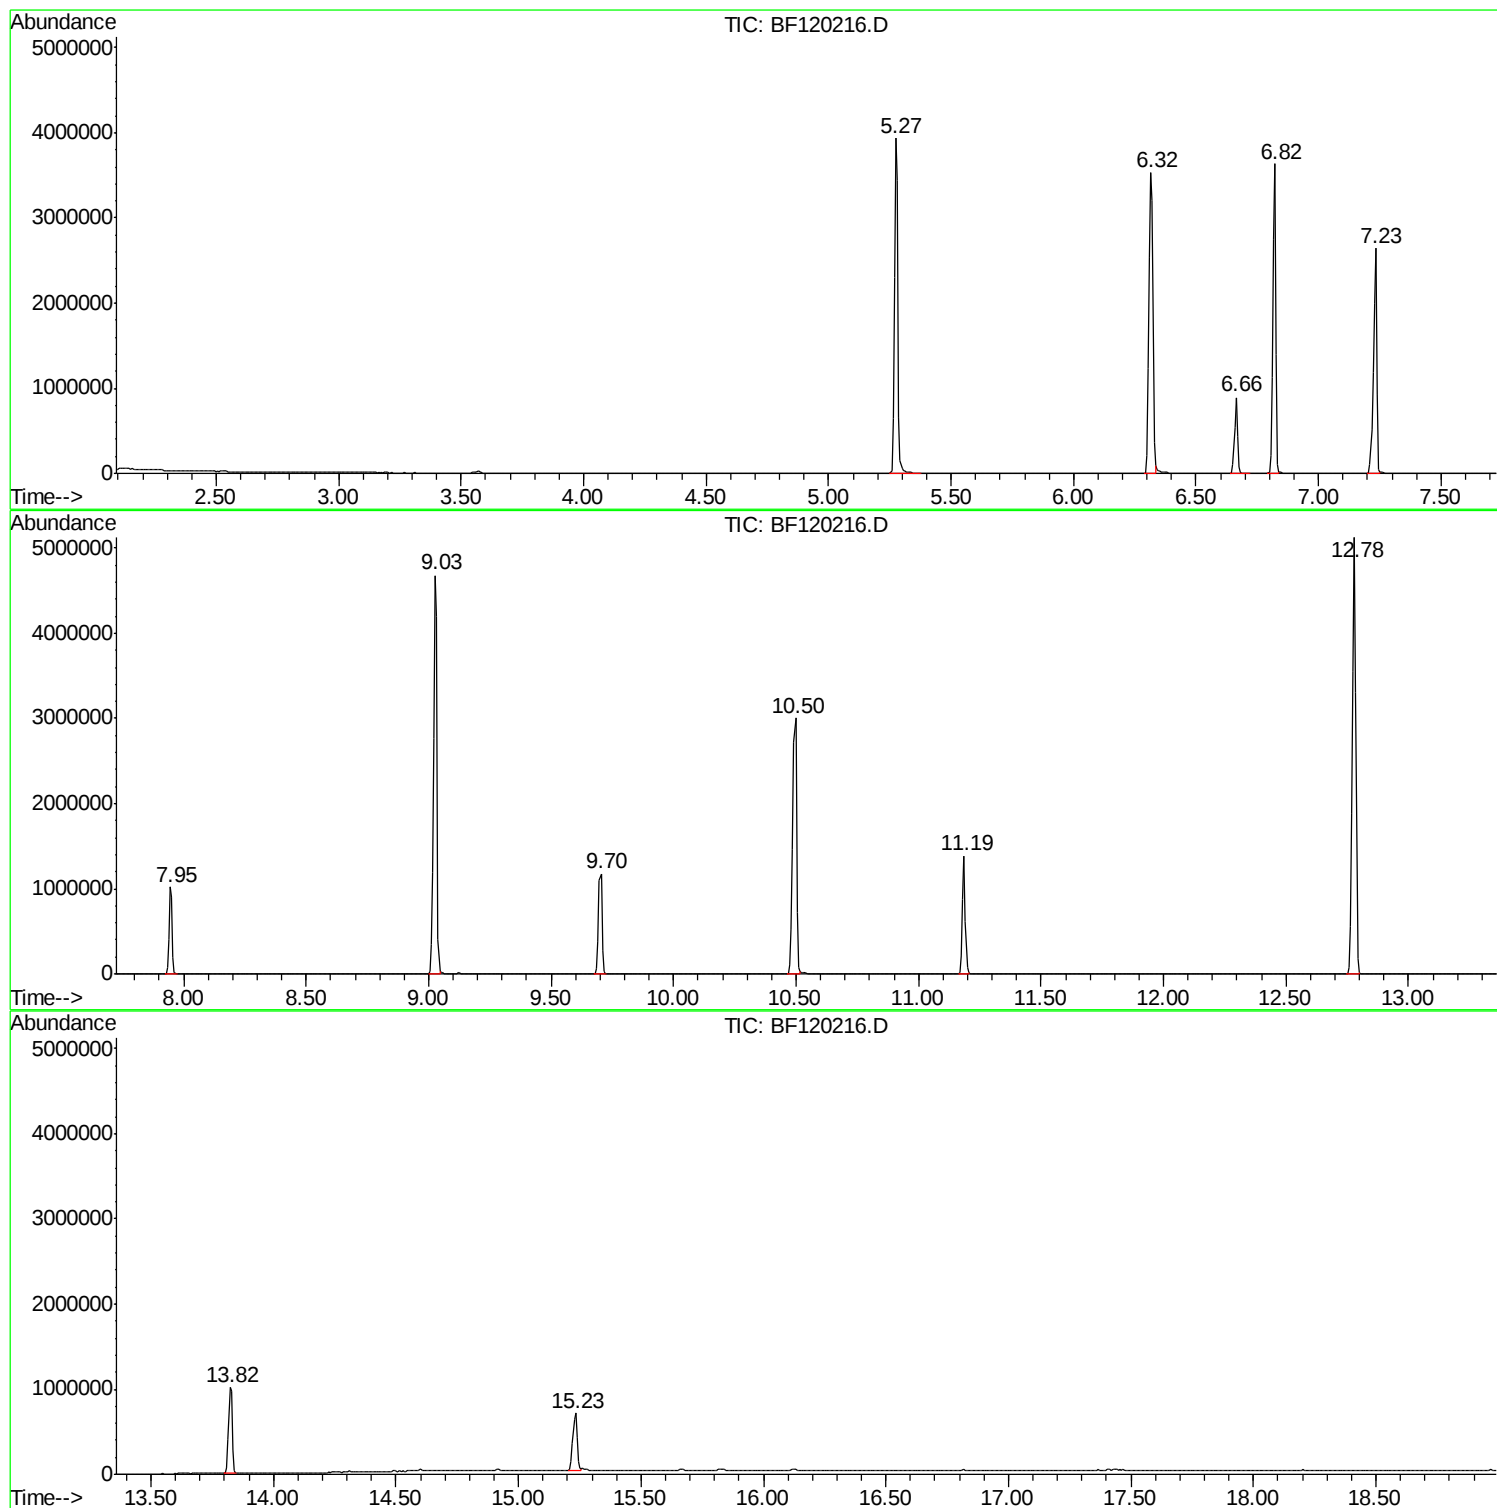

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042720\
Data_File : BF120216.D
Acq_On : 27 Apr 2020 14:011
Operator : MA/SJJ
Sample : PB128487BLL
Misc :
ALS_Vial : 7 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128487BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
