

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042720\
 Data File : BF120219.D
 Acq On : 27 Apr 2020 15:22
 Operator : MA/SJ
 Sample : L2375-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-16A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.451	57	62	69	rVB	410020	513799	8.43%	1.374%
2	4.187	352	357	366	rVB	58008	77406	1.27%	0.207%
3	4.398	388	393	400	rVB	133478	154206	2.53%	0.412%
4	4.869	469	473	481	rVB	157673	169403	2.78%	0.453%
5	5.287	539	544	557	rBV	3932120	3966246	65.07%	10.606%
6	6.316	715	719	737	rBV	3114056	3380627	55.46%	9.040%
7	6.498	746	750	758	rBV	51552	69783	1.14%	0.187%
8	6.663	774	778	782	rBV	933204	720519	11.82%	1.927%
9	6.822	800	805	808	rBV	3716166	3289314	53.96%	8.796%
10	7.233	869	875	878	rBV	3052220	3125252	51.27%	8.357%
11	7.945	992	996	998	rBV	1231077	1063244	17.44%	2.843%
12	7.969	998	1000	1004	rVB	446930	335299	5.50%	0.897%
13	8.663	1114	1118	1122	rBV	134589	119649	1.96%	0.320%
14	8.757	1130	1134	1138	rBV	135404	113842	1.87%	0.304%
15	9.027	1175	1180	1183	rBV	5612936	5676996	93.13%	15.181%
16	9.698	1290	1294	1297	rBV	1304113	1195353	19.61%	3.197%
17	9.733	1297	1300	1308	rVB	140563	121715	2.00%	0.325%
18	10.498	1424	1430	1433	rBV	3491403	3610432	59.23%	9.655%
19	11.186	1543	1547	1549	rBV	1410356	1244584	20.42%	3.328%
20	11.210	1549	1551	1554	rVB	129699	102756	1.69%	0.275%
21	11.721	1635	1638	1643	rBV2	151259	165532	2.72%	0.443%
22	12.510	1769	1772	1786	rBV2	104094	178008	2.92%	0.476%
23	12.780	1812	1818	1821	rBV	5547201	6095684	100.00%	16.301%
24	13.821	1991	1995	1999	rBV	1109436	1034882	16.98%	2.767%
25	15.227	2229	2234	2238	rBV	704887	870843	14.29%	2.329%


Sum of corrected areas: 37395374

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042720\
Data File : BF120219.D
Acq On : 27 Apr 2020 15:22
Operator : MA/SJ
Sample : L2375-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-16A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

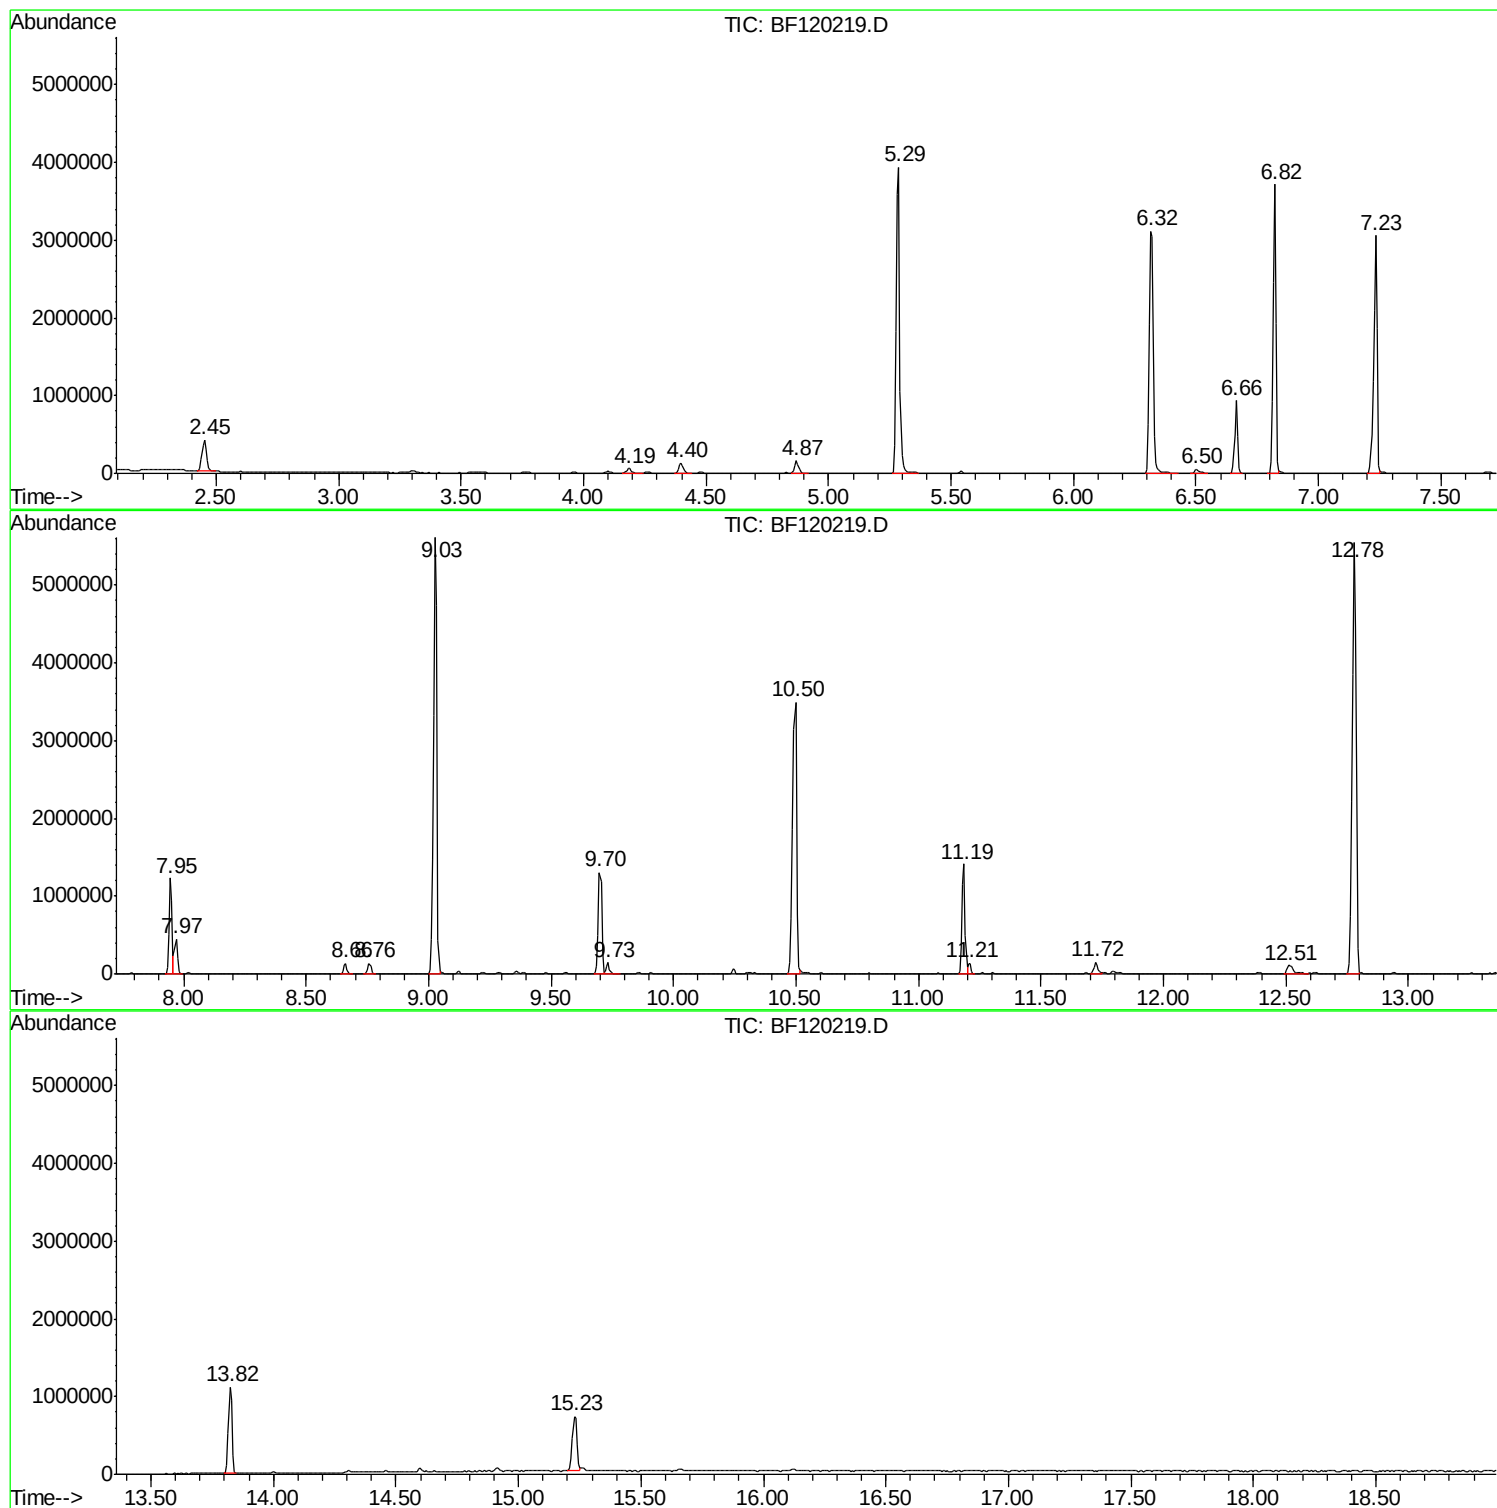

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042720\
Data_File : BF120219.D
Acq_On : 27 Apr 2020 15:222
Operator : MA/SJJ
Sample : L2375-044
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
TP-16A

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
