


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042720\
 Data File : BF120210.D
 Acq On : 27 Apr 2020 11:11
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 27 12:17:15 2020

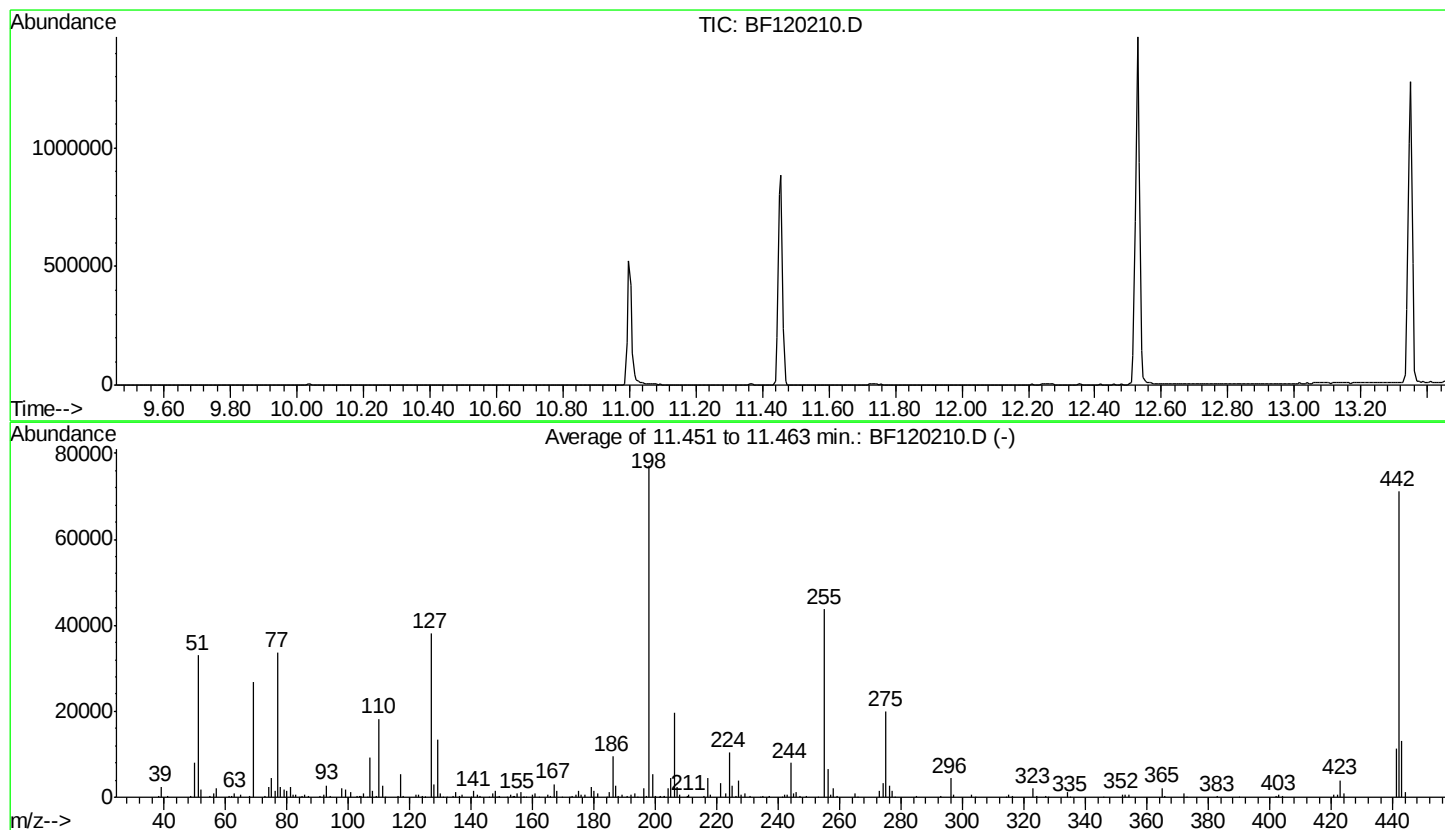

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	33021	PASS
68	69	0.00	2	1.6	422	PASS
69	198	0.00	100	34.6	26707	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	38105	PASS
197	198	0.00	2	0.4	283	PASS
198	198	100	100	100.0	77125	PASS
199	198	5	9	6.9	5342	PASS
275	198	10	60	25.7	19845	PASS
365	198	1	100	2.9	2225	PASS
441	198	0.01	100	14.5	11218	PASS
442	198	50	100	92.1	71016	PASS
443	442	15	24	18.6	13191	PASS