

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF043020\
 Data File : BF120240.D
 Acq On : 30 Apr 2020 15:19
 Operator : MA/SJ
 Sample : PB128574BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128574BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.251	535	538	551	rBV	2952304	2927660	73.19%	12.353%
2	6.298	712	716	729	rBV	2891678	2902730	72.57%	12.248%
3	6.645	772	775	787	rBV	588065	511851	12.80%	2.160%
4	6.804	798	802	805	rBV	2976654	2373249	59.33%	10.013%
5	7.216	867	872	875	rBV	2094342	1794094	44.85%	7.570%
6	7.933	990	994	1001	rBV	825054	657874	16.45%	2.776%
7	9.016	1174	1178	1181	rBV	3837174	3222234	80.55%	13.596%
8	9.692	1289	1293	1296	rBV	853816	751064	18.78%	3.169%
9	10.480	1423	1427	1431	rBV	2422067	2255027	56.37%	9.515%
10	11.174	1541	1545	1549	rBV	1010293	798652	19.97%	3.370%
11	12.768	1811	1816	1819	rBV	4007969	4000106	100.00%	16.878%
12	13.815	1990	1994	1999	rBV	904992	779961	19.50%	3.291%
13	15.221	2228	2233	2237	rBV	621645	726027	18.15%	3.063%


Sum of corrected areas: 23700529

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF043020\
Data File : BF120240.D
Acq On : 30 Apr 2020 15:19
Operator : MA/SJ
Sample : PB128574BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128574BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

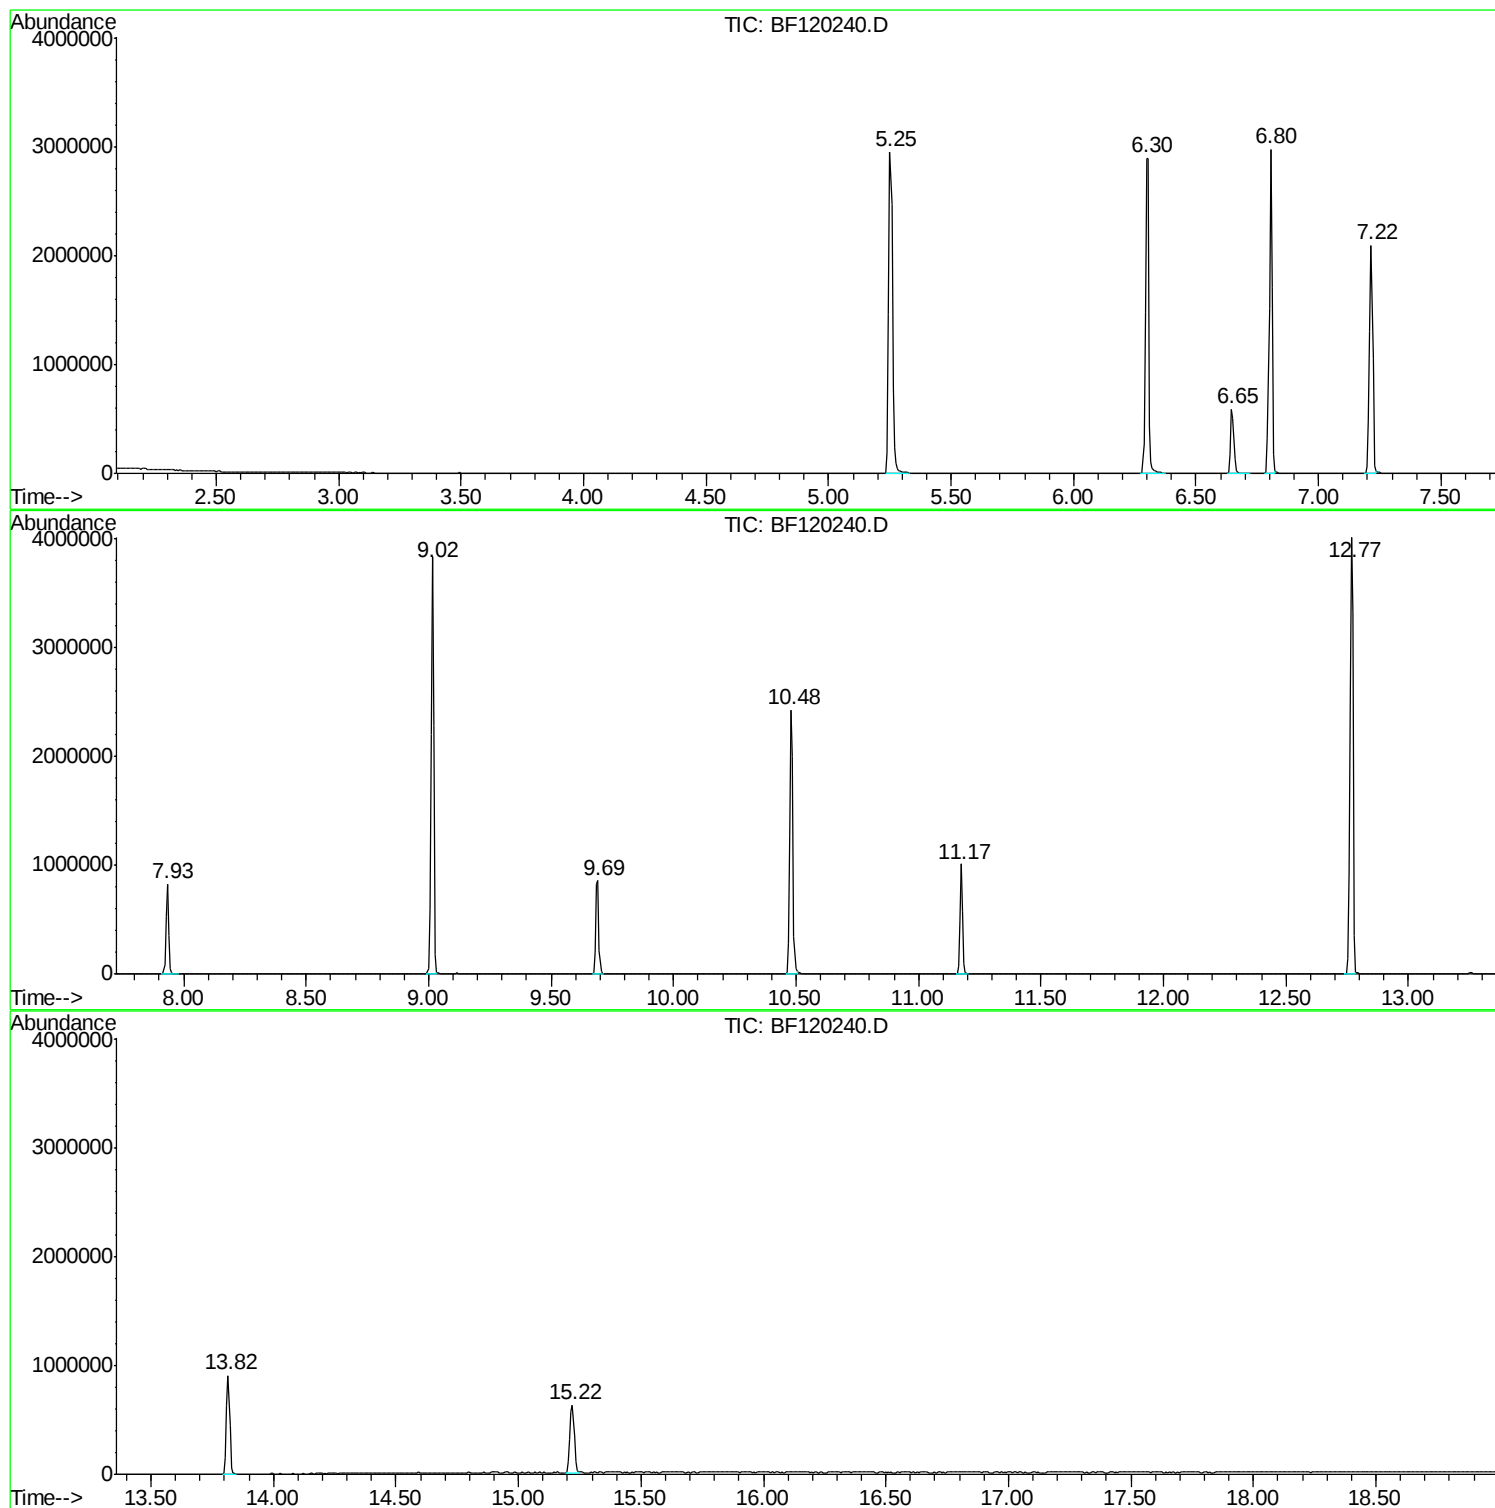

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF043020\
Data File : BF120240.D
Acq On : 30 Apr 2020 15:19
Operator : MA/SJ
Sample : PB128574BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128574BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF043020\
Data File : BF120240.D
Acq On : 30 Apr 2020 15:19
Operator : MA/SJ
Sample : PB128574BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128574BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc