


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF043020\
 Data File : BF120232.D
 Acq On : 30 Apr 2020 11:39
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 12:39:25 2020

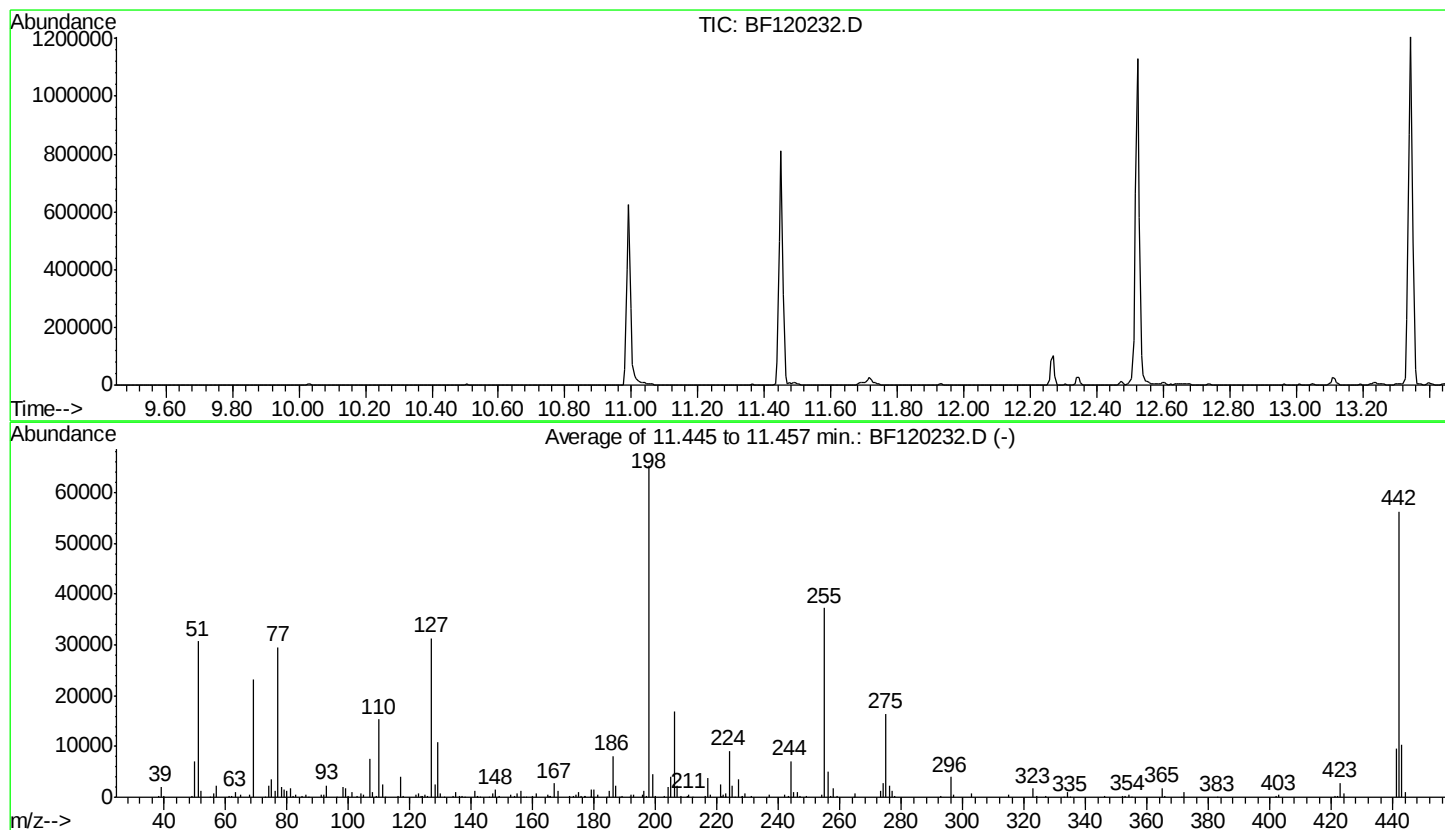

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	30716	PASS
68	69	0.00	2	1.7	401	PASS
69	198	0.00	100	35.6	23252	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	31381	PASS
197	198	0.00	2	0.2	146	PASS
198	198	100	100	100.0	65354	PASS
199	198	5	9	6.8	4461	PASS
275	198	10	60	25.2	16493	PASS
365	198	1	100	2.8	1834	PASS
441	198	0.01	100	14.5	9482	PASS
442	198	50	100	86.1	56264	PASS
443	442	15	24	18.5	10434	PASS