

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114062.D
 Acq On : 1 May 2019 12:09
 Operator : JU/SJ
 Sample : K2194-05RE 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-CRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	578	582	595	rBV	987101	992472	5.74%	1.202%
2	6.516	749	753	771	rBV	1168352	1141115	6.60%	1.383%
3	6.663	774	778	785	rBV	1531413	1191953	6.89%	1.444%
4	6.892	814	817	825	rBV	818867	696105	4.02%	0.843%
5	7.051	840	844	847	rBV	1177459	935833	5.41%	1.134%
6	7.451	904	912	917	rBV	790613	773929	4.47%	0.938%
7	8.175	1030	1035	1042	rBV	1009652	1110247	6.42%	1.345%
8	8.769	1133	1136	1140	rBV2	320728	309402	1.79%	0.375%
9	9.133	1194	1198	1202	rVB2	109916	200451	1.16%	0.243%
10	9.198	1207	1209	1214	rVB2	240440	262902	1.52%	0.319%
11	9.251	1214	1218	1221	rBV	1679971	1393300	8.05%	1.688%
12	9.333	1229	1232	1237	rBV	662118	600460	3.47%	0.728%
13	9.404	1241	1244	1247	rVB2	193742	184723	1.07%	0.224%
14	9.575	1269	1273	1274	rBV2	158508	180382	1.04%	0.219%
15	9.657	1282	1287	1289	rVV4	475906	699476	4.04%	0.847%
16	9.680	1289	1291	1293	rVV2	243246	242363	1.40%	0.294%
17	9.716	1293	1297	1299	rVV	273581	308421	1.78%	0.374%
18	9.863	1315	1322	1325	rBV	1059583	1035045	5.98%	1.254%
19	9.904	1327	1329	1331	rBV3	156844	175865	1.02%	0.213%
20	9.933	1331	1334	1337	rVB	1314318	1140818	6.59%	1.382%
21	10.039	1349	1352	1357	rBV4	172762	184055	1.06%	0.223%
22	10.098	1359	1362	1364	rVV2	181679	259774	1.50%	0.315%
23	10.127	1364	1367	1370	rVV4	223804	343622	1.99%	0.416%
24	10.186	1373	1377	1381	rVV5	347628	465943	2.69%	0.565%
25	10.251	1385	1388	1391	rBV3	180492	241586	1.40%	0.293%
26	10.363	1401	1407	1410	rBV	1276901	1159800	6.70%	1.405%
27	10.427	1415	1418	1422	rVB4	142104	186048	1.08%	0.225%
28	10.586	1439	1445	1450	rBV	536255	752709	4.35%	0.912%
29	10.722	1465	1468	1471	rVB	931513	838833	4.85%	1.016%
30	10.839	1485	1488	1497	rVB	1213213	1619177	9.36%	1.962%
31	11.063	1524	1526	1529	rVB2	218033	186911	1.08%	0.226%
32	11.286	1560	1564	1566	rBV	1194040	936952	5.42%	1.135%
33	11.316	1566	1569	1575	rVB	647462	690841	3.99%	0.837%
34	11.422	1583	1587	1589	rBV	1139894	1096723	6.34%	1.329%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114062.D
 Acq On : 1 May 2019 12:09
 Operator : JU/SJ
 Sample : K2194-05RE 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-CRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.439	1589	1590	1593	rVV	632682	543531	3.14%	0.659%
36	11.492	1597	1599	1603	rVB	301504	289925	1.68%	0.351%
37	11.710	1633	1636	1638	rBV	1062113	852202	4.93%	1.033%
38	11.733	1638	1640	1642	rVB2	378578	266088	1.54%	0.322%
39	11.816	1649	1654	1657	rBV	7553483	8685213	50.20%	10.523%
40	11.874	1662	1664	1669	rVV2	135047	178918	1.03%	0.217%
41	11.921	1669	1672	1674	rVV	220754	228693	1.32%	0.277%
42	11.951	1674	1677	1682	rVB	1007626	1083849	6.26%	1.313%
43	12.033	1688	1691	1694	rBV	359146	370748	2.14%	0.449%
44	12.121	1702	1706	1710	rVB	794121	840966	4.86%	1.019%
45	12.216	1719	1722	1724	rBV2	313561	263526	1.52%	0.319%
46	12.521	1766	1774	1775	rBV2	8175571	17302345	100.00%	20.963%
47	12.610	1786	1789	1791	rVV	4766899	3914857	22.63%	4.743%
48	12.639	1791	1794	1796	rVV	2107789	2273655	13.14%	2.755%
49	12.669	1796	1799	1805	rVV	2404132	3672856	21.23%	4.450%
50	12.739	1808	1811	1815	rVB2	489443	569129	3.29%	0.690%
51	12.839	1824	1828	1830	rBV	1070921	1065491	6.16%	1.291%
52	12.874	1830	1834	1841	rVB2	1697797	2350010	13.58%	2.847%
53	12.933	1841	1844	1846	rVB2	183505	188740	1.09%	0.229%
54	13.010	1853	1857	1859	rVB	1604972	1513859	8.75%	1.834%
55	13.045	1859	1863	1866	rVB3	169509	213776	1.24%	0.259%
56	13.086	1867	1870	1872	rBV3	232246	293500	1.70%	0.356%
57	13.163	1880	1883	1885	rBV	1063012	963522	5.57%	1.167%
58	13.251	1893	1898	1904	rVB3	1020336	1769286	10.23%	2.144%
59	13.298	1904	1906	1908	rBV2	198793	216699	1.25%	0.263%
60	13.327	1908	1911	1915	rVB	965279	812553	4.70%	0.984%
61	13.427	1925	1928	1930	rBV2	177282	218982	1.27%	0.265%
62	13.574	1951	1953	1956	rBV	391930	309438	1.79%	0.375%
63	13.745	1980	1982	1986	rBV2	203562	257775	1.49%	0.312%
64	13.910	2007	2010	2014	rBV3	364747	327129	1.89%	0.396%
65	13.998	2022	2025	2030	rVB	612793	522803	3.02%	0.633%
66	14.068	2032	2037	2040	rBV2	1415216	2013211	11.64%	2.439%
67	14.092	2040	2041	2044	rVB	630928	509493	2.94%	0.617%
68	14.233	2062	2065	2068	rVB	395514	368156	2.13%	0.446%
69	14.551	2116	2119	2125	rBV4	469556	729774	4.22%	0.884%
70	14.639	2132	2134	2137	rBV	192942	179042	1.03%	0.217%
71	14.868	2170	2173	2176	rBV	356158	352225	2.04%	0.427%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data File : BF114062.D
Acq On : 1 May 2019 12:09
Operator : JU/SJ
Sample : K2194-05RE 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-CRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.986	2188	2193	2201	rVB	763589	1139089	6.58%	1.380%
73	15.145	2216	2220	2222	rBV	477851	689800	3.99%	0.836%
74	15.215	2229	2232	2235	rVB2	367742	410732	2.37%	0.498%
75	15.515	2280	2283	2289	rVB	514550	669767	3.87%	0.811%
76	15.580	2291	2294	2296	rBV	486517	577722	3.34%	0.700%


Sum of corrected areas: 82537311

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
Data File : BF114062.D
Acq On : 1 May 2019 12:09
Operator : JU/SJ
Sample : K2194-05RE 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-CRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

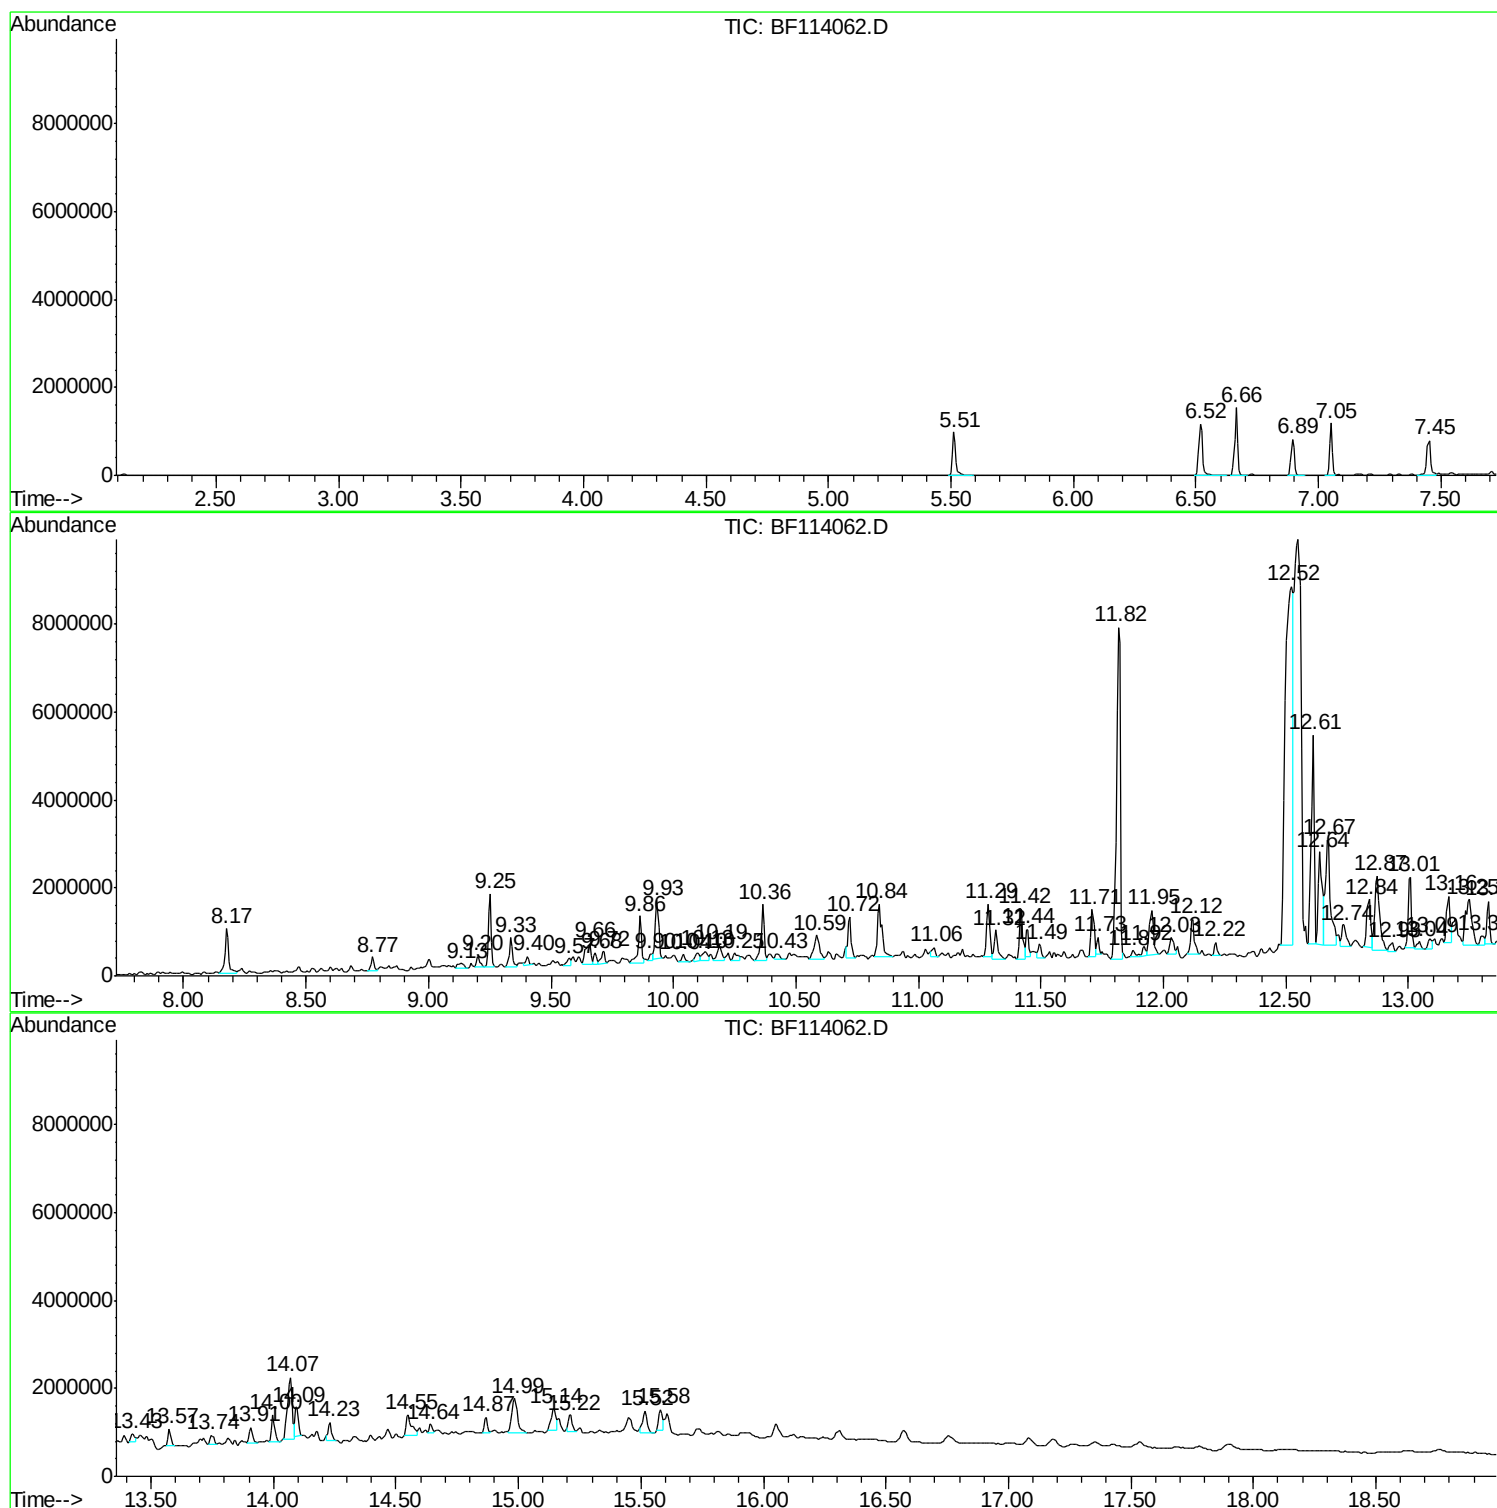

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data_File : BF114062.D
Acq_On : 1_May, 2019 12:099
Operator : JU/SJJ
Sample : K2194-05RE_2XX
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-CRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
