

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114065.D
 Acq On : 1 May 2019 13:28
 Operator : JU/SJ
 Sample : K2194-11RE 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-FRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	579	583	598	rBV	1155985	1074586	2.23%	0.827%
2	6.522	750	754	773	rBV	1305388	1190236	2.47%	0.916%
3	6.663	775	778	782	rBV	1335926	1235615	2.57%	0.951%
4	6.898	814	818	821	rBV	742052	636421	1.32%	0.490%
5	7.051	840	844	848	rBV	1168260	975999	2.03%	0.751%
6	7.451	904	912	917	rBV	839473	782904	1.63%	0.603%
7	8.163	1030	1033	1034	rVV	803797	677607	1.41%	0.522%
8	8.180	1034	1036	1042	rVV	994209	964095	2.00%	0.742%
9	8.774	1133	1137	1141	rBV	1230848	1131840	2.35%	0.871%
10	9.139	1194	1199	1203	rVB3	306690	487989	1.01%	0.376%
11	9.251	1215	1218	1223	rVB	1830348	1587553	3.30%	1.222%
12	9.339	1229	1233	1237	rBV	1794745	1532934	3.19%	1.180%
13	9.657	1282	1287	1289	rVV4	742748	1095250	2.28%	0.843%
14	9.869	1316	1323	1326	rBV	2064299	1867148	3.88%	1.437%
15	9.939	1331	1335	1338	rVB	1066118	1087802	2.26%	0.837%
16	10.192	1374	1378	1382	rBV5	457847	714252	1.48%	0.550%
17	10.368	1402	1408	1411	rBV	2283172	2076782	4.32%	1.599%
18	10.586	1440	1445	1450	rBV	764427	1135073	2.36%	0.874%
19	10.721	1466	1468	1472	rVB	877752	772077	1.60%	0.594%
20	10.839	1485	1488	1498	rBV	1980800	2554196	5.31%	1.966%
21	11.286	1561	1564	1567	rBV	1770394	1642346	3.41%	1.264%
22	11.321	1567	1570	1575	rVB	855829	924276	1.92%	0.711%
23	11.421	1584	1587	1590	rBV	1058681	1047864	2.18%	0.807%
24	11.715	1634	1637	1639	rBV	1772020	1542479	3.20%	1.187%
25	11.733	1639	1640	1645	rVB2	712979	555388	1.15%	0.428%
26	11.833	1650	1657	1659	rBV	8383696	12437087	25.84%	9.574%
27	11.968	1674	1680	1685	rBV	1159706	1726662	3.59%	1.329%
28	12.121	1700	1706	1711	rBV	1533755	1703680	3.54%	1.311%
29	12.574	1766	1783	1786	rBV5	9854414	48129084	100.00%	37.049%
30	12.598	1786	1787	1788	rVV	1204181	585996	1.22%	0.451%
31	12.627	1788	1792	1794	rVV	6891887	6839518	14.21%	5.265%
32	12.692	1794	1803	1807	rVV	3985811	8240005	17.12%	6.343%
33	12.751	1810	1813	1817	rVB	780021	814958	1.69%	0.627%
34	12.845	1826	1829	1833	rVB	1778066	1628298	3.38%	1.253%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
Data File : BF114065.D
Acq On : 1 May 2019 13:28
Operator : JU/SJ
Sample : K2194-11RE 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-FRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.886	1833	1836	1839	rBV2	1097849	1001289	2.08%	0.771%
36	13.015	1855	1858	1861	rVB	1625309	1424695	2.96%	1.097%
37	13.168	1881	1884	1886	rBV	1496138	1325059	2.75%	1.020%
38	13.192	1886	1888	1894	rVB3	469267	729432	1.52%	0.562%
39	13.257	1894	1899	1902	rBV2	1557443	2150080	4.47%	1.655%
40	13.333	1908	1912	1915	rBV	1615792	1436613	2.98%	1.106%
41	13.439	1927	1930	1932	rBV3	580866	482576	1.00%	0.371%
42	13.515	1941	1943	1946	rVB2	586347	531379	1.10%	0.409%
43	13.580	1949	1954	1958	rVB	720661	735823	1.53%	0.566%
44	13.751	1980	1983	1987	rVB3	357733	488462	1.01%	0.376%
45	14.004	2023	2026	2034	rVB	1279845	1129142	2.35%	0.869%
46	14.074	2035	2038	2041	rBV	937532	851042	1.77%	0.655%
47	14.233	2062	2065	2068	rBV	616896	573821	1.19%	0.442%
48	14.551	2115	2119	2126	rBV	985422	1442886	3.00%	1.111%
49	14.645	2132	2135	2138	rBV	574491	526038	1.09%	0.405%
50	14.868	2170	2173	2176	rBV	553339	500679	1.04%	0.385%
51	14.986	2189	2193	2203	rVB	897620	1530558	3.18%	1.178%
52	15.215	2229	2232	2236	rVB	555951	629541	1.31%	0.485%
53	15.586	2292	2295	2297	rBV	362210	492529	1.02%	0.379%
54	16.056	2372	2375	2383	rVB	384782	527845	1.10%	0.406%


Sum of corrected areas: 129907489

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
Data File : BF114065.D
Acq On : 1 May 2019 13:28
Operator : JU/SJ
Sample : K2194-11RE 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-FRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

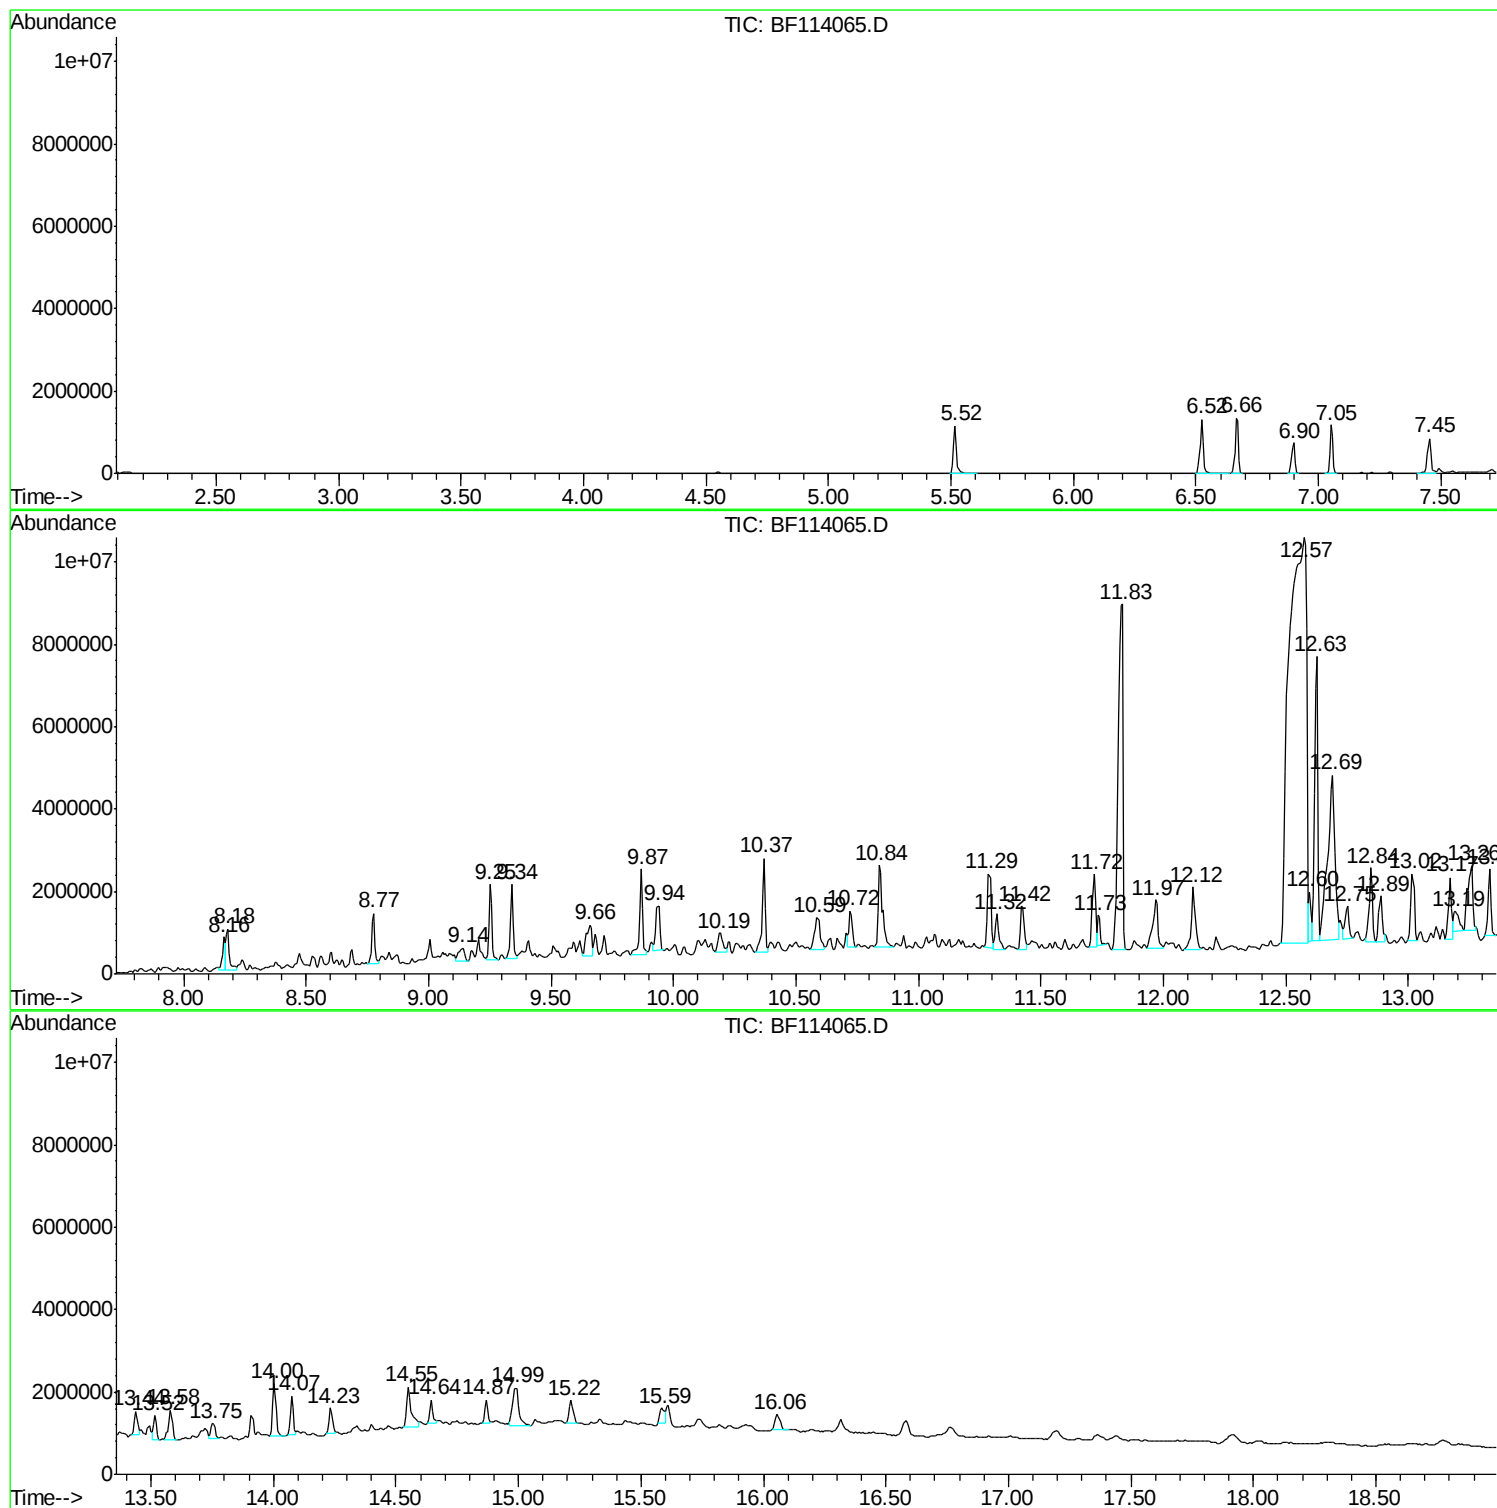

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data_File : BF114065.D
Acq_On : 1_May, 2019 13:288
Operator : JU/SJJ
Sample : K2194-11RE_2XX
Misc :
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-FRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
