

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114066.D
 Acq On : 1 May 2019 13:55
 Operator : JU/SJ
 Sample : K2194-13RE 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-GRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	579	583	600	rVB	835976	853428	3.88%	1.111%
2	6.522	750	754	771	rVB	1257032	1129303	5.14%	1.470%
3	6.663	775	778	782	rBV	1297737	1152346	5.25%	1.500%
4	6.898	814	818	823	rBV	629452	543127	2.47%	0.707%
5	7.051	841	844	848	rBV	939606	809904	3.69%	1.054%
6	7.451	904	912	917	rBV	676943	648790	2.95%	0.844%
7	8.163	1030	1033	1034	rBV	515737	401957	1.83%	0.523%
8	8.181	1034	1036	1039	rVV	721727	628993	2.86%	0.819%
9	8.239	1042	1046	1049	rVB2	175243	231494	1.05%	0.301%
10	8.475	1080	1086	1090	rBV4	219491	273415	1.24%	0.356%
11	8.686	1118	1122	1125	rBV	282664	258247	1.18%	0.336%
12	8.775	1133	1137	1141	rBV	768295	710109	3.23%	0.924%
13	9.139	1194	1199	1203	rVB2	180691	308795	1.41%	0.402%
14	9.204	1207	1210	1215	rVV4	271285	332435	1.51%	0.433%
15	9.251	1215	1218	1224	rVB	1436236	1181594	5.38%	1.538%
16	9.339	1229	1233	1237	rBV	1043649	931911	4.24%	1.213%
17	9.510	1257	1262	1268	rVB8	165793	254990	1.16%	0.332%
18	9.592	1268	1276	1278	rBV6	236794	452646	2.06%	0.589%
19	9.657	1282	1287	1289	rVV4	462109	679058	3.09%	0.884%
20	9.680	1289	1291	1294	rVV2	282936	279827	1.27%	0.364%
21	9.716	1294	1297	1300	rVV	293726	256185	1.17%	0.333%
22	9.869	1320	1323	1326	rVB	1085748	814043	3.71%	1.059%
23	9.939	1331	1335	1338	rVB	979175	926101	4.22%	1.205%
24	10.098	1359	1362	1365	rBV3	181446	264031	1.20%	0.344%
25	10.186	1374	1377	1382	rBV5	291329	434979	1.98%	0.566%
26	10.369	1402	1408	1410	rBV	1254876	1115532	5.08%	1.452%
27	10.586	1440	1445	1451	rBV	433880	639127	2.91%	0.832%
28	10.722	1466	1468	1472	rVB	692822	616194	2.80%	0.802%
29	10.839	1485	1488	1496	rVB	1173478	1348395	6.14%	1.755%
30	11.286	1561	1564	1567	rBV	1054607	880711	4.01%	1.146%
31	11.316	1567	1569	1575	rVB	482243	554777	2.53%	0.722%
32	11.421	1584	1587	1590	rBV	894438	842229	3.83%	1.096%
33	11.716	1634	1637	1639	rBV	1074866	903951	4.11%	1.176%
34	11.733	1639	1640	1643	rVB	486096	294422	1.34%	0.383%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114066.D
 Acq On : 1 May 2019 13:55
 Operator : JU/SJ
 Sample : K2194-13RE 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-GRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.821	1650	1655	1658	rBV	7271584	8963143	40.80%	11.665%
36	11.957	1674	1678	1685	rVV	751582	949650	4.32%	1.236%
37	12.121	1701	1706	1711	rVB2	823932	858214	3.91%	1.117%
38	12.527	1767	1775	1777	rBV2	8632492	21969845	100.00%	28.593%
39	12.616	1786	1790	1792	rVB	4853136	4175432	19.01%	5.434%
40	12.680	1792	1801	1806	rBV3	2364411	4725186	21.51%	6.150%
41	12.739	1809	1811	1816	rVB2	411878	420818	1.92%	0.548%
42	12.839	1825	1828	1832	rVV	996727	990983	4.51%	1.290%
43	12.880	1832	1835	1842	rVB2	625016	759588	3.46%	0.989%
44	13.010	1854	1857	1860	rBV	1404865	1206477	5.49%	1.570%
45	13.163	1881	1883	1885	rBV	749637	700784	3.19%	0.912%
46	13.192	1885	1888	1893	rVV3	512476	932997	4.25%	1.214%
47	13.251	1893	1898	1905	rVB2	1040694	1684040	7.67%	2.192%
48	13.327	1908	1911	1915	rVB	885290	848895	3.86%	1.105%
49	13.433	1924	1929	1932	rBV4	364540	534468	2.43%	0.696%
50	13.510	1940	1942	1946	rVB3	296878	344660	1.57%	0.449%
51	13.580	1951	1954	1957	rVB	395798	341073	1.55%	0.444%
52	13.751	1980	1983	1987	rVB3	316509	408939	1.86%	0.532%
53	13.910	2007	2010	2012	rBV	279659	220878	1.01%	0.287%
54	13.998	2022	2025	2033	rVB	757813	735164	3.35%	0.957%
55	14.068	2034	2037	2040	rBV	706744	707924	3.22%	0.921%
56	14.227	2062	2064	2073	rBV	290222	323352	1.47%	0.421%
57	14.545	2115	2118	2120	rBV	539284	575668	2.62%	0.749%
58	14.633	2131	2133	2136	rBV2	278047	246347	1.12%	0.321%
59	14.857	2169	2171	2175	rVB	287778	254425	1.16%	0.331%
60	14.980	2188	2192	2194	rBV	562136	642583	2.92%	0.836%
61	15.574	2290	2293	2295	rBV	287782	362778	1.65%	0.472%


Sum of corrected areas: 76837357

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
Data File : BF114066.D
Acq On : 1 May 2019 13:55
Operator : JU/SJ
Sample : K2194-13RE 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-GRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

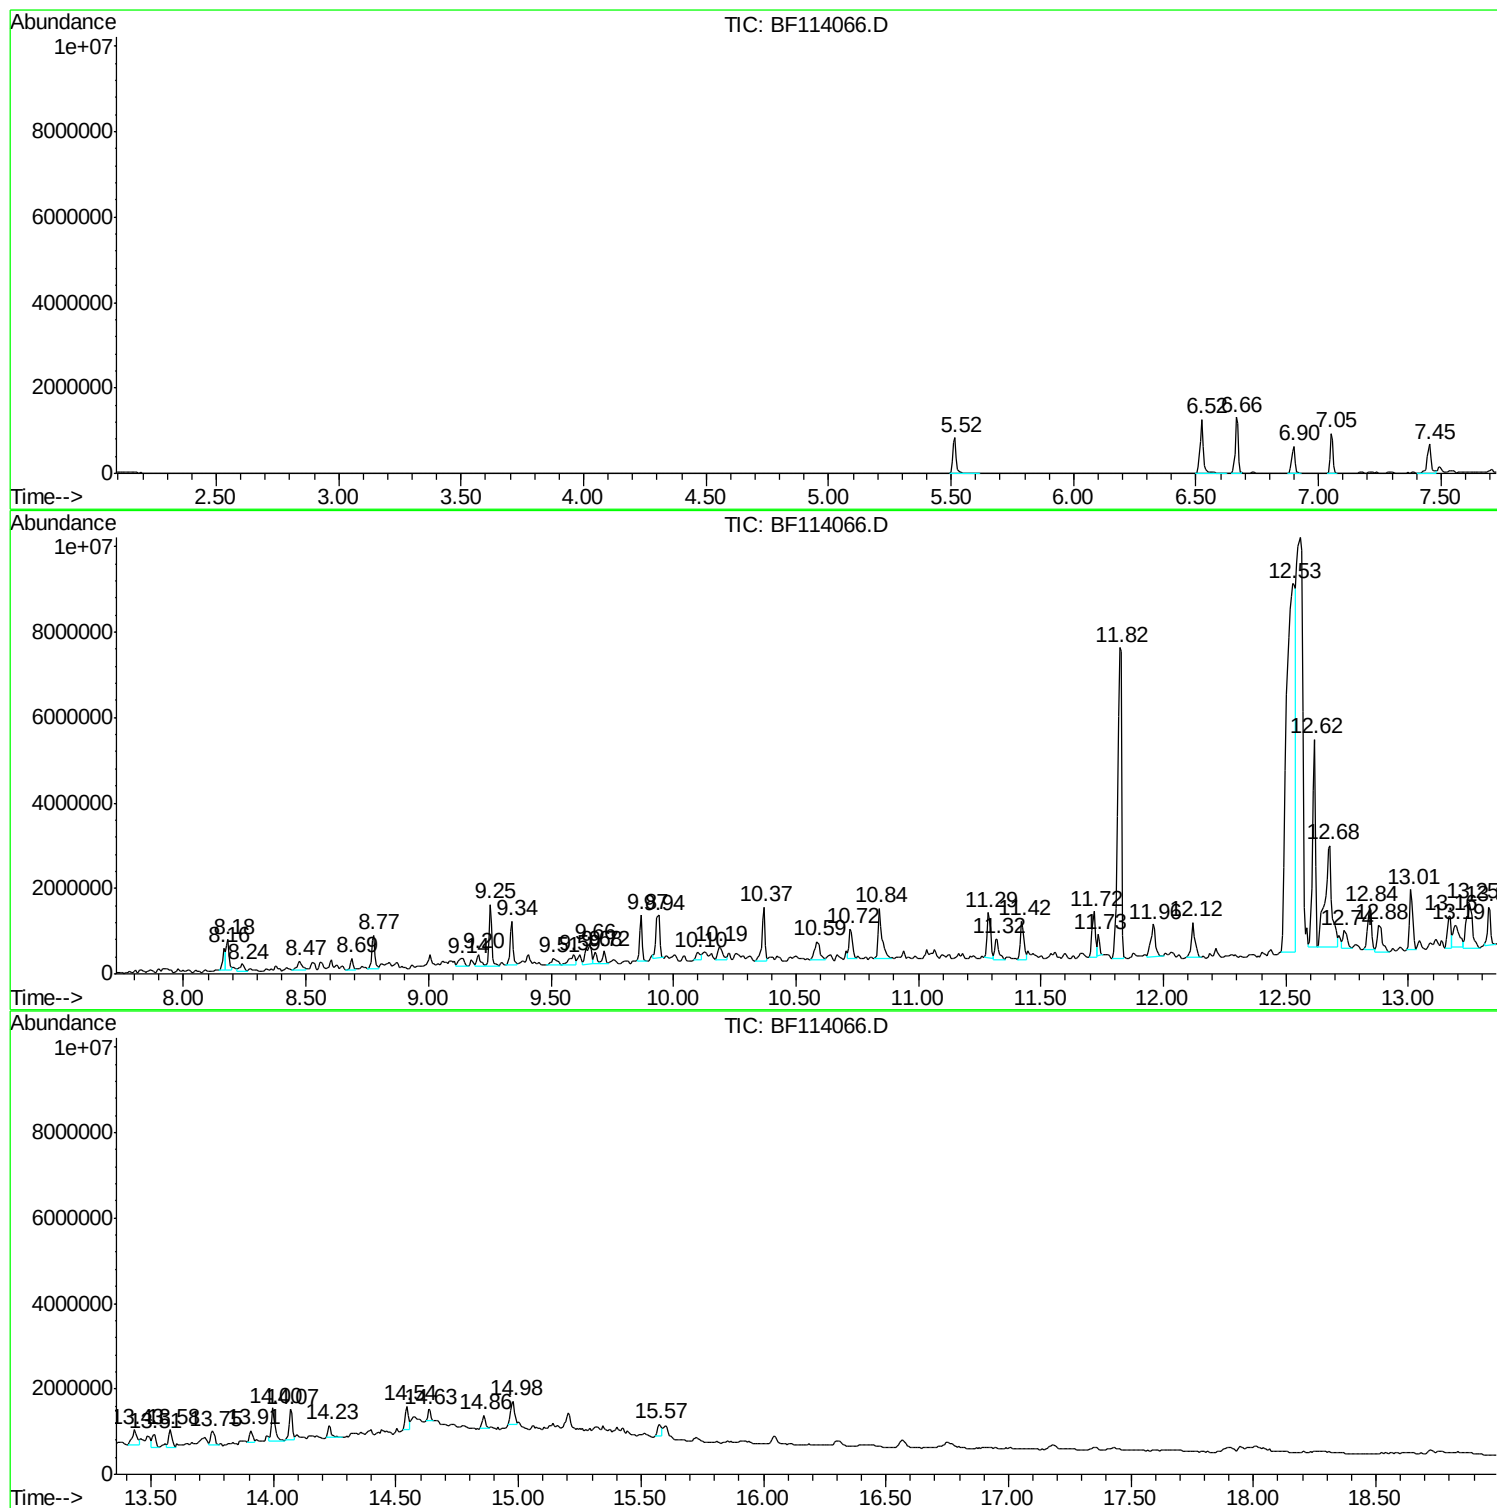

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data_File : BF114066.D
Acq_On : 1_May_2019_ 13:555
Operator : JU/SJJ
Sample : K2194-13RE_2XX
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-GRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
