

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114067.D
 Acq On : 1 May 2019 14:21
 Operator : JU/SJ
 Sample : K2194-17RE 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-IRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	580	583	597	rVB	723089	715590	16.00%	2.699%
2	6.522	750	754	764	rBV	850258	795261	17.78%	2.999%
3	6.669	775	779	786	rBV	933707	826063	18.47%	3.115%
4	6.898	814	818	825	rBV	664856	533456	11.93%	2.012%
5	7.051	841	844	848	rBV	733867	648895	14.51%	2.447%
6	7.451	908	912	924	rBV	594374	517336	11.57%	1.951%
7	8.180	1031	1036	1044	rBV	778574	729856	16.32%	2.752%
8	9.251	1215	1218	1224	rBV	1190327	995611	22.26%	3.755%
9	9.333	1229	1232	1236	rBV	109015	114245	2.55%	0.431%
10	9.580	1269	1274	1275	rBV5	33506	49269	1.10%	0.186%
11	9.645	1282	1285	1289	rBV2	154507	200256	4.48%	0.755%
12	9.716	1294	1297	1300	rVB2	60440	51428	1.15%	0.194%
13	9.798	1308	1311	1315	rBV4	36692	48794	1.09%	0.184%
14	9.863	1319	1322	1326	rVB	160773	153051	3.42%	0.577%
15	9.939	1331	1335	1338	rVV	851169	778065	17.39%	2.934%
16	10.045	1349	1353	1358	rBV7	40371	54973	1.23%	0.207%
17	10.098	1358	1362	1365	rBV3	54912	91587	2.05%	0.345%
18	10.186	1374	1377	1382	rBV6	74614	108186	2.42%	0.408%
19	10.257	1386	1389	1391	rBV3	40507	51982	1.16%	0.196%
20	10.363	1402	1407	1410	rBV	307134	291898	6.53%	1.101%
21	10.586	1439	1445	1450	rBV	144778	223196	4.99%	0.842%
22	10.669	1457	1459	1463	rBV2	42738	48435	1.08%	0.183%
23	10.721	1463	1468	1472	rBV	683817	658492	14.72%	2.483%
24	10.839	1485	1488	1496	rVB	361133	448337	10.02%	1.691%
25	11.063	1524	1526	1529	rVB3	66298	54005	1.21%	0.204%
26	11.286	1561	1564	1567	rBV	358685	296122	6.62%	1.117%
27	11.316	1567	1569	1575	rVB	172448	201982	4.52%	0.762%
28	11.421	1584	1587	1590	rBV	948250	874290	19.55%	3.297%
29	11.445	1590	1591	1594	rVV	203333	156689	3.50%	0.591%
30	11.498	1598	1600	1604	rVV	69785	65315	1.46%	0.246%
31	11.592	1614	1616	1620	rVB3	60404	50972	1.14%	0.192%
32	11.716	1633	1637	1639	rBV	301574	279456	6.25%	1.054%
33	11.810	1650	1653	1656	rVB	760714	581357	13.00%	2.192%
34	11.945	1673	1676	1683	rVB2	470297	500597	11.19%	1.888%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
 Data File : BF114067.D
 Acq On : 1 May 2019 14:21
 Operator : JU/SJ
 Sample : K2194-17RE 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-03-042919-IRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.121	1703	1706	1710	rVB	239897	224772	5.02%	0.848%
36	12.498	1766	1770	1772	rBV	2668118	2616197	58.49%	9.866%
37	12.521	1772	1774	1780	rVB	4692556	4473190	100.00%	16.869%
38	12.604	1784	1788	1791	rBV	795524	699334	15.63%	2.637%
39	12.639	1791	1794	1795	rBV	492442	447169	10.00%	1.686%
40	12.657	1795	1797	1807	rVV	682427	985655	22.03%	3.717%
41	12.733	1807	1810	1817	rVB2	188158	211216	4.72%	0.797%
42	12.839	1825	1828	1830	rBV	137765	133755	2.99%	0.504%
43	12.868	1830	1833	1840	rVB2	227833	368790	8.24%	1.391%
44	13.004	1853	1856	1859	rBV	1128452	975327	21.80%	3.678%
45	13.110	1872	1874	1876	rBV2	61832	47372	1.06%	0.179%
46	13.133	1876	1878	1880	rBV2	76833	53925	1.21%	0.203%
47	13.162	1880	1883	1885	rBV	248817	199270	4.45%	0.751%
48	13.192	1885	1888	1891	rVB3	88524	104597	2.34%	0.394%
49	13.239	1893	1896	1897	rBV	187353	199404	4.46%	0.752%
50	13.327	1909	1911	1915	rVB	190371	162970	3.64%	0.615%
51	13.580	1952	1954	1957	rBV	138513	126009	2.82%	0.475%
52	13.915	2009	2011	2013	rBV	110568	87545	1.96%	0.330%
53	14.009	2024	2027	2031	rBV	129823	154615	3.46%	0.583%
54	14.080	2035	2039	2041	rBV2	758295	795594	17.79%	3.000%
55	14.245	2065	2067	2068	rBV	140066	76255	1.70%	0.288%
56	15.162	2220	2223	2228	rBV2	201107	392443	8.77%	1.480%
57	15.227	2231	2234	2238	rVB2	295531	345037	7.71%	1.301%
58	15.598	2294	2297	2300	rBV	361664	441167	9.86%	1.664%


Sum of corrected areas: 26516655

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
Data File : BF114067.D
Acq On : 1 May 2019 14:21
Operator : JU/SJ
Sample : K2194-17RE 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-IRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

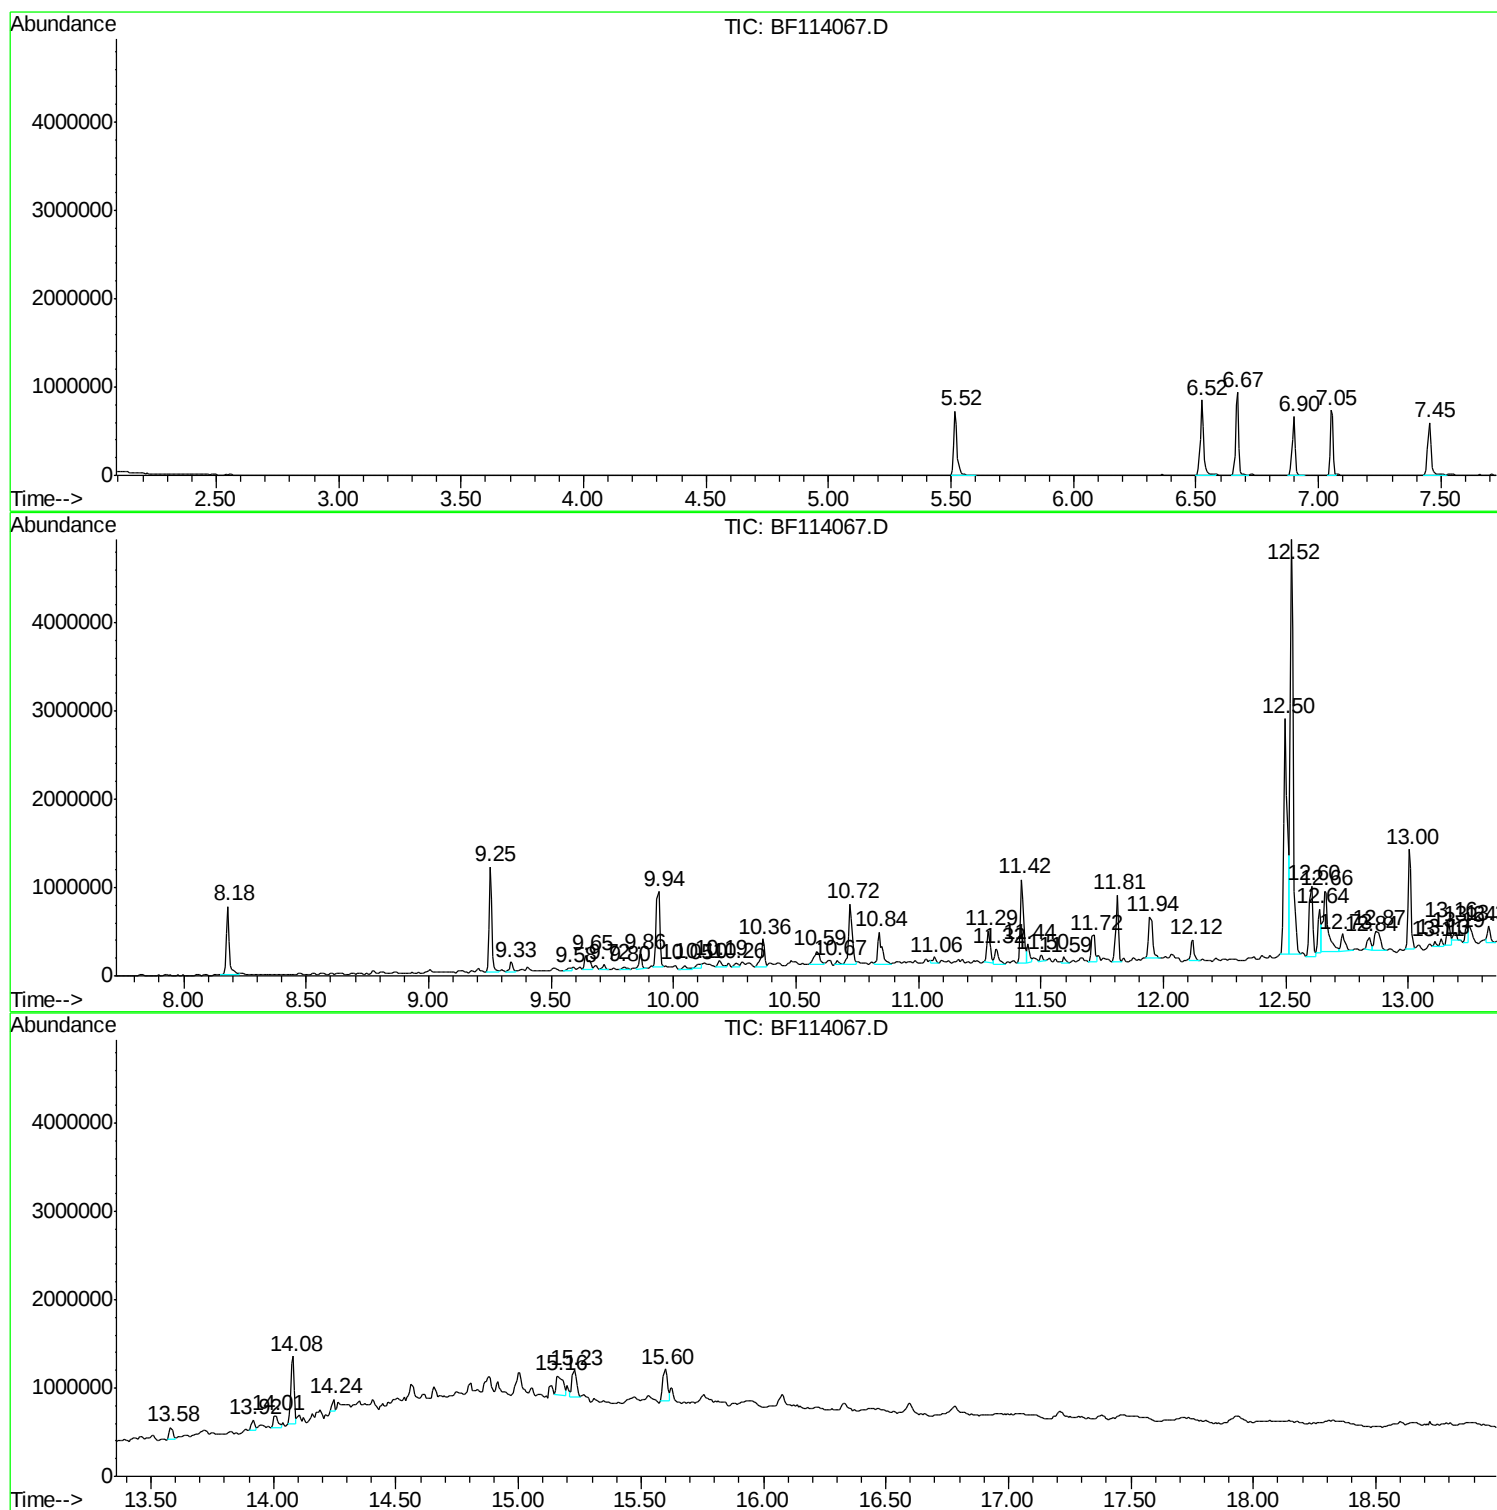

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data_File : BF114067.D
Acq_On : 1_May, 2019 14:211
Operator : JU/SJJ
Sample : K2194-17RE_2XX
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
JC-03-042919-IRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
