

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114074.D
 Acq On : 1 May 2019 17:47
 Operator : JU/SJ
 Sample : K2191-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P-66-TPRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	3	7	11	rVB	29071	37138	2.13%	0.220%
2	5.516	579	583	598	rVB	1516810	1398313	80.05%	8.269%
3	6.440	737	740	746	rVB	30495	29752	1.70%	0.176%
4	6.528	750	755	767	rVV	1435502	1478237	84.63%	8.741%
5	6.669	774	779	782	rBV	1666595	1546586	88.54%	9.145%
6	6.893	814	817	821	rBV	529521	471295	26.98%	2.787%
7	7.051	840	844	848	rBV	1416948	1185584	67.87%	7.011%
8	7.451	908	912	924	rBV	969330	888456	50.86%	5.254%
9	8.181	1032	1036	1043	rBV	665532	616816	35.31%	3.647%
10	9.134	1193	1198	1203	rBV	35472	64155	3.67%	0.379%
11	9.251	1214	1218	1225	rBV	2064811	1746752	100.00%	10.329%
12	9.334	1229	1232	1239	rVV6	20136	38469	2.20%	0.227%
13	9.392	1239	1242	1247	rVB	47444	53287	3.05%	0.315%
14	9.639	1281	1284	1290	rVB	207516	184176	10.54%	1.089%
15	9.804	1309	1312	1315	rBV6	14471	20521	1.17%	0.121%
16	9.851	1317	1320	1324	rVB2	39850	42339	2.42%	0.250%
17	9.934	1331	1334	1339	rVB	924610	775732	44.41%	4.587%
18	10.722	1464	1468	1476	rBV	1299727	1204739	68.97%	7.124%
19	10.833	1482	1487	1489	rBV2	22209	38010	2.18%	0.225%
20	11.016	1515	1518	1523	rBV	24977	26444	1.51%	0.156%
21	11.422	1583	1587	1594	rBV	942568	818831	46.88%	4.842%
22	11.945	1673	1676	1686	rBV	182910	188846	10.81%	1.117%
23	12.727	1806	1809	1812	rBV4	43992	50183	2.87%	0.297%
24	13.004	1852	1856	1859	rBV	1968192	1631062	93.38%	9.645%
25	13.692	1971	1973	1976	rVB4	52031	37866	2.17%	0.224%
26	13.910	2007	2010	2023	rBV4	153910	393016	22.50%	2.324%
27	14.063	2033	2036	2040	rBV	755233	742524	42.51%	4.391%
28	14.221	2061	2063	2067	rBV2	50238	50605	2.90%	0.299%
29	14.345	2082	2084	2087	rBV	73264	59289	3.39%	0.351%
30	14.533	2114	2116	2119	rBV	105702	93715	5.37%	0.554%
31	14.845	2167	2169	2175	rVB	85010	95412	5.46%	0.564%
32	15.198	2225	2229	2237	rVB	128796	179319	10.27%	1.060%
33	15.563	2287	2291	2302	rVB	475884	723659	41.43%	4.279%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data File : BF114074.D
Acq On : 1 May 2019 17:47
Operator : JU/SJ
Sample : K2191-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P-66-TPRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 16911128

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF050119\
Data File : BF114074.D
Acq On : 1 May 2019 17:47
Operator : JU/SJ
Sample : K2191-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P-66-TPRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

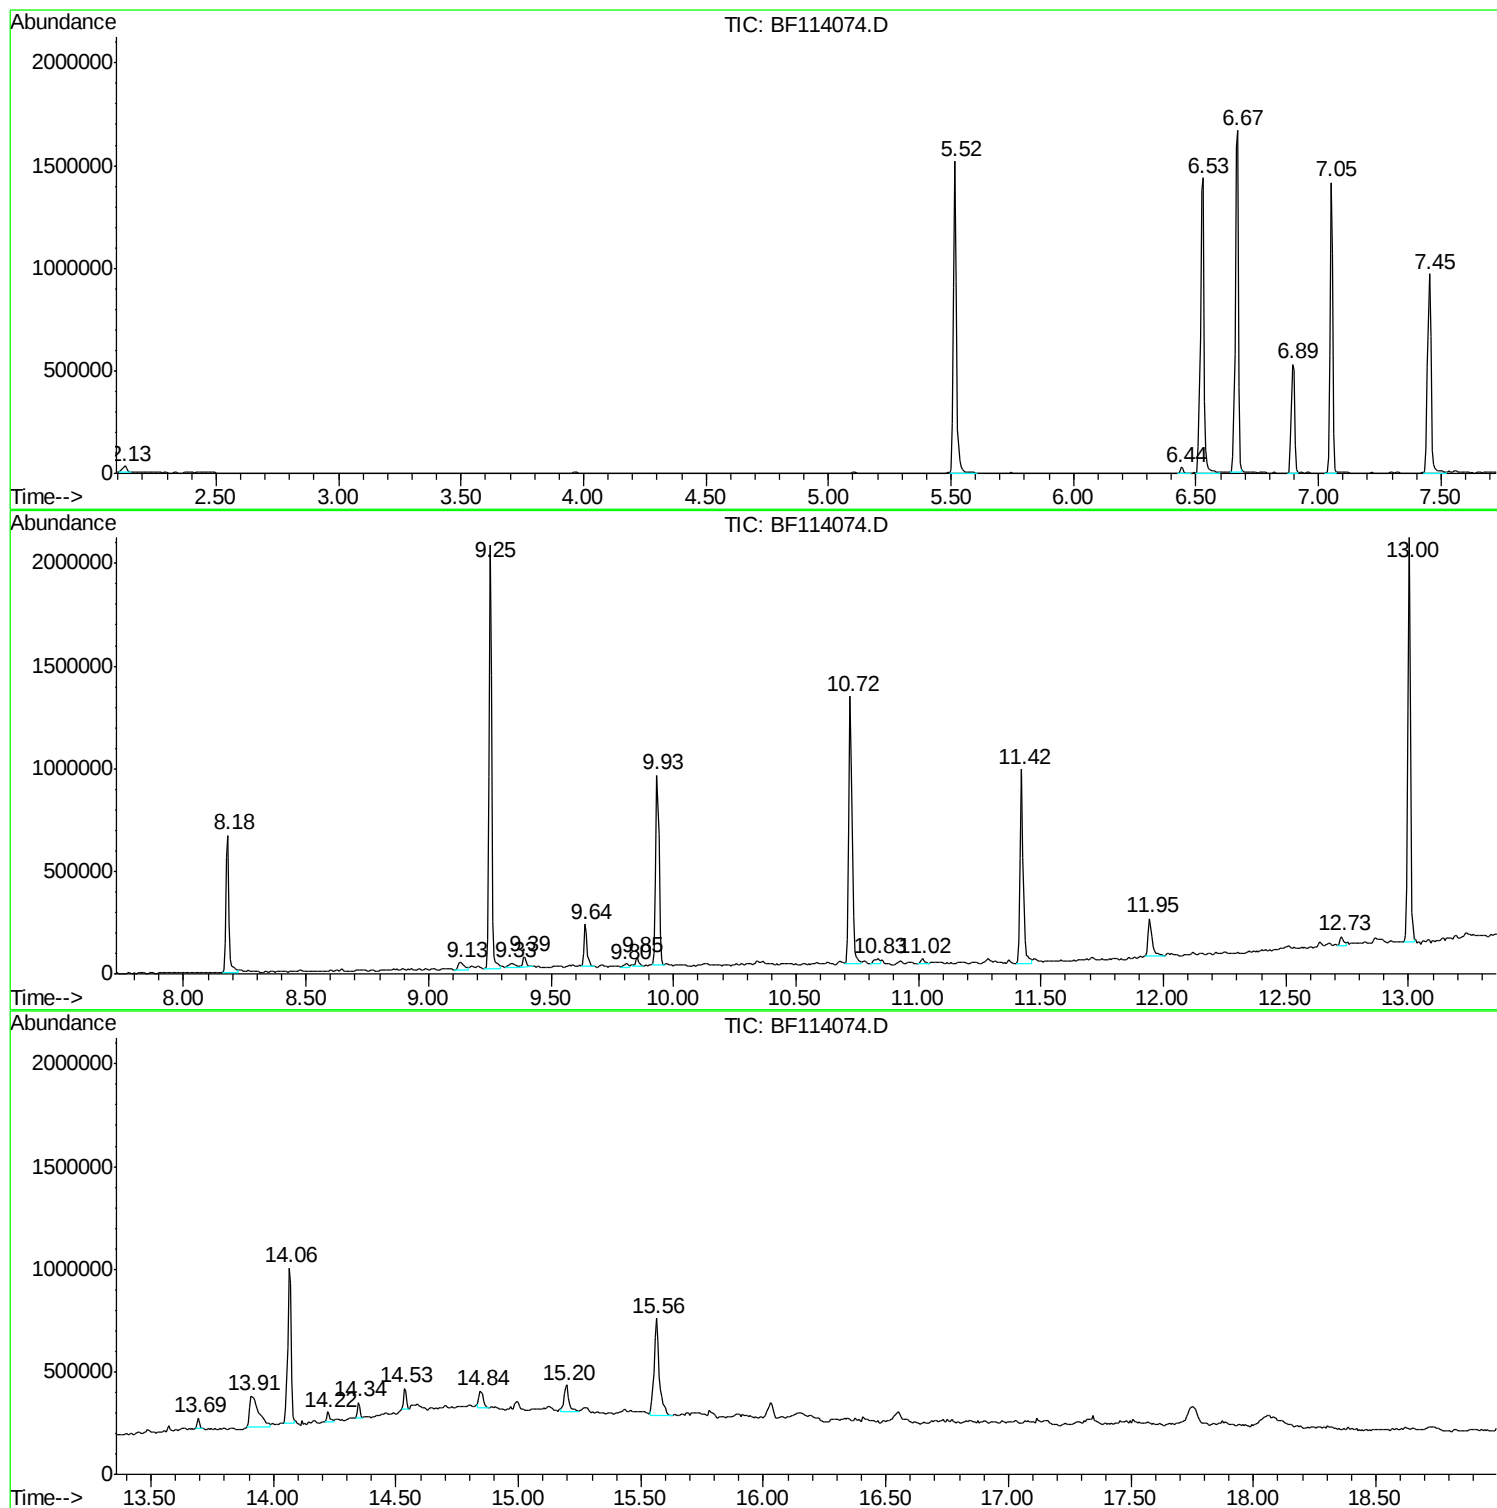

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
Data_File : BF114074.D
Acq_On : 1_May, 2019 17:477
Operator : JU/SJJ
Sample : K2191-01REE
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
P-66-TPRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
