


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050119\
 Data File : BF114057.D
 Acq On : 1 May 2019 9:48
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

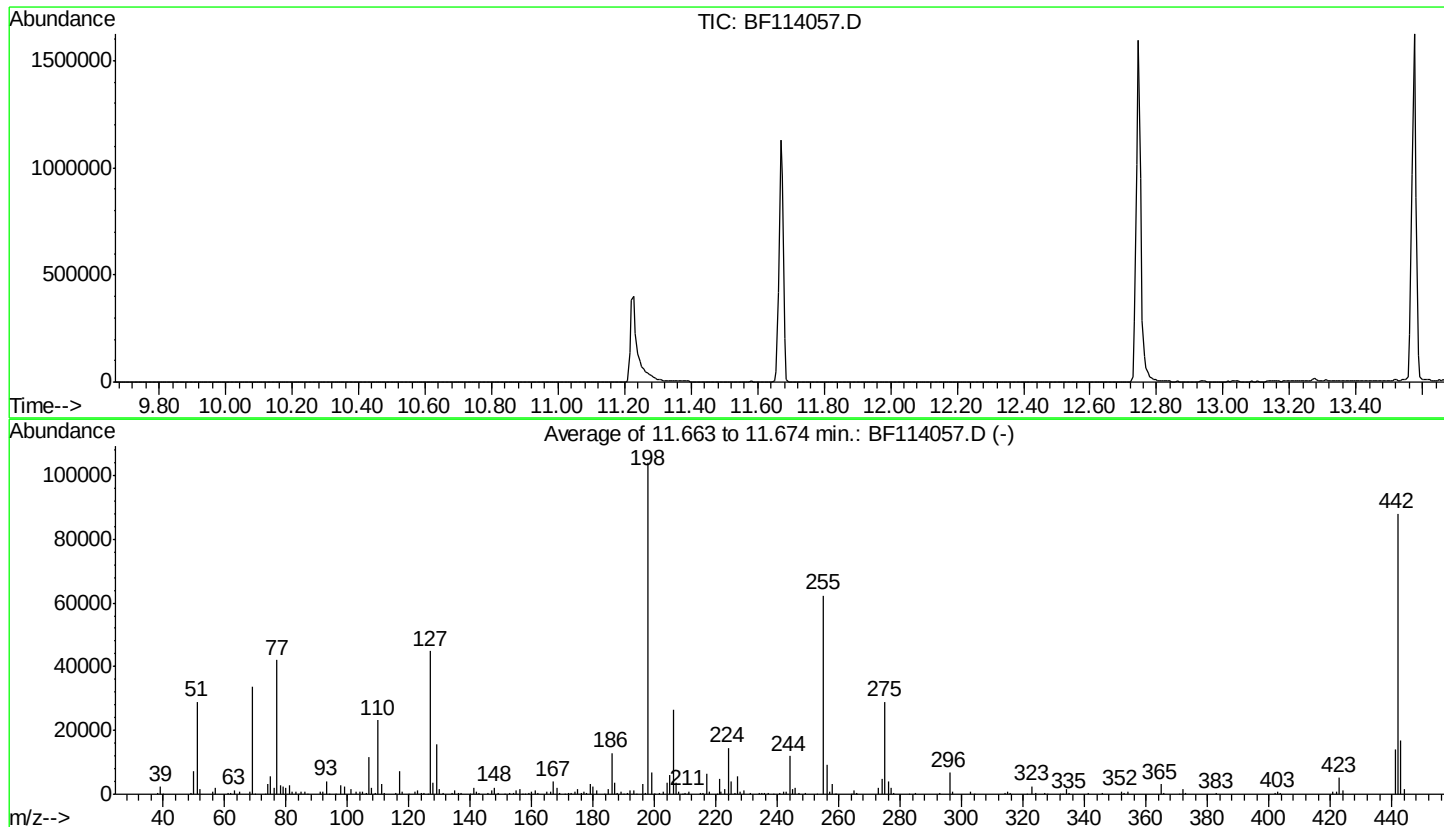

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	28981	PASS
68	69	0.00	2	1.9	626	PASS
69	198	0.00	100	32.3	33600	PASS
70	69	0.00	2	0.4	126	PASS
127	198	10	80	43.2	44914	PASS
197	198	0.00	2	0.5	545	PASS
198	198	100	100	100.0	103984	PASS
199	198	5	9	6.7	6994	PASS
275	198	10	60	27.8	28931	PASS
365	198	1	100	3.1	3186	PASS
441	198	0.01	100	13.6	14173	PASS
442	198	50	100	84.7	88114	PASS
443	442	15	24	19.2	16943	PASS