
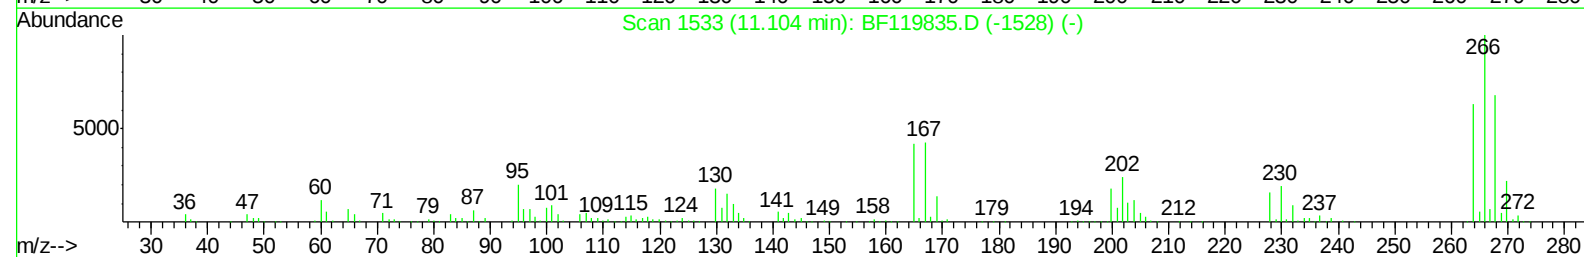
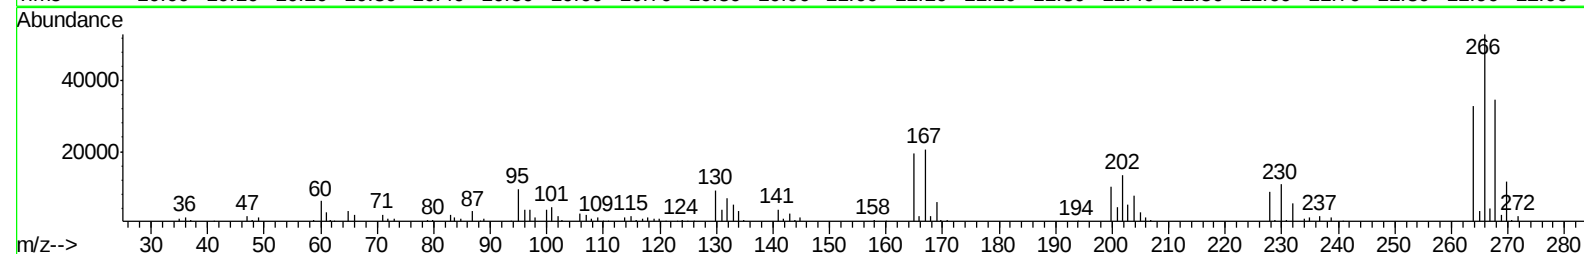


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF050120\
 Data File : BF120256.D
 Acq On : 1 May 2020 13:20
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 04:38:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 01 15:26:36 2020
 Response via : Initial Calibration

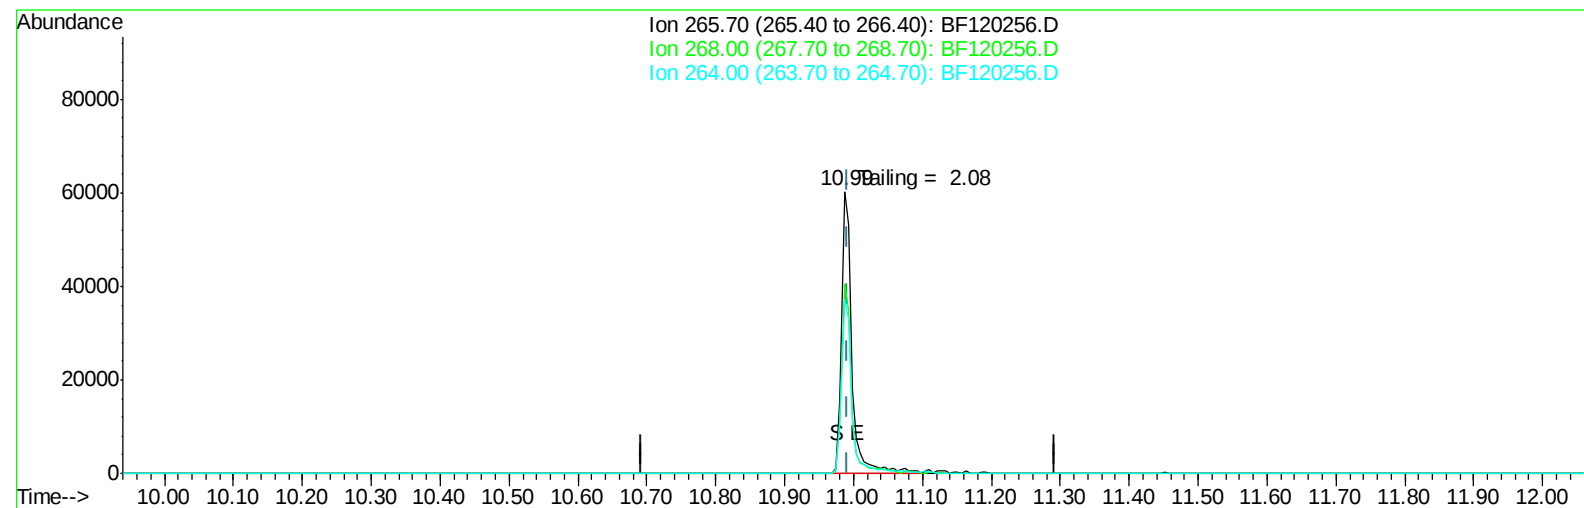

TIC: BF120256.D

(70) Pentachlorophenol (C)




10.986min (-0.006) 57286.02ng

response 60390

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.41
264.00	61.20	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF050120\
 Data File : BF120256.D
 Acq On : 1 May 2020 13:20
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 04:38:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 01 15:26:36 2020
 Response via : Initial Calibration

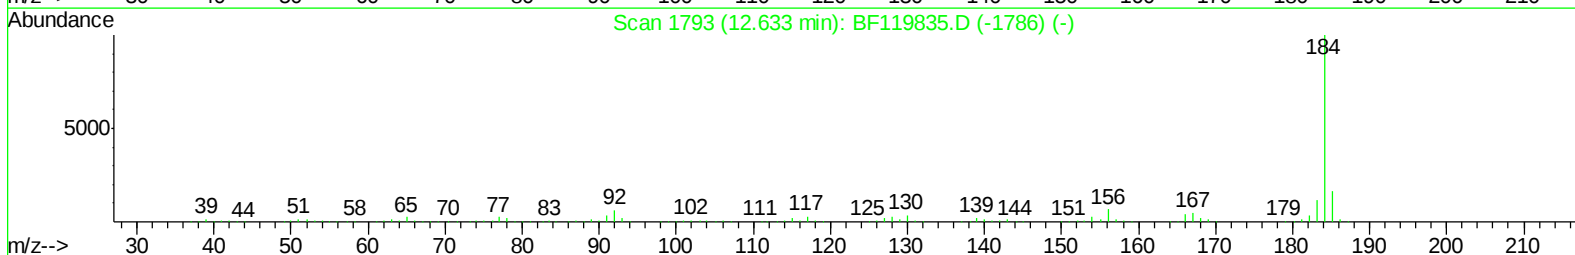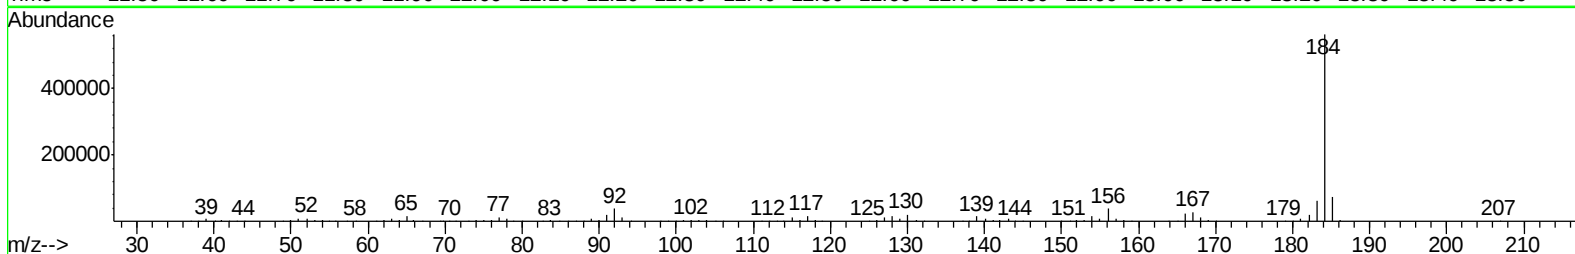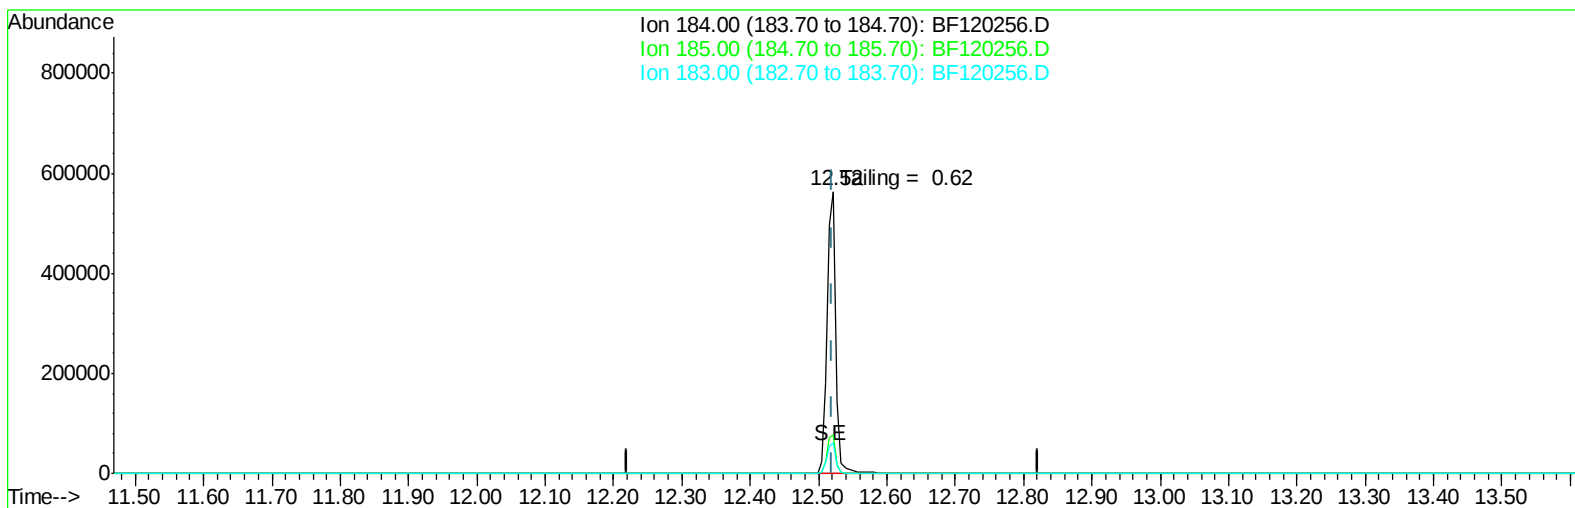

TIC: BF120256.D

(77) Benzidine

12.522min (+0.000) 0.00ng

response 517506

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.42
183.00	11.30	10.76
0.00	0.00	0.00