


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF050120\
 Data File : BF120256.D
 Acq On : 1 May 2020 13:20
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 01 15:26:36 2020

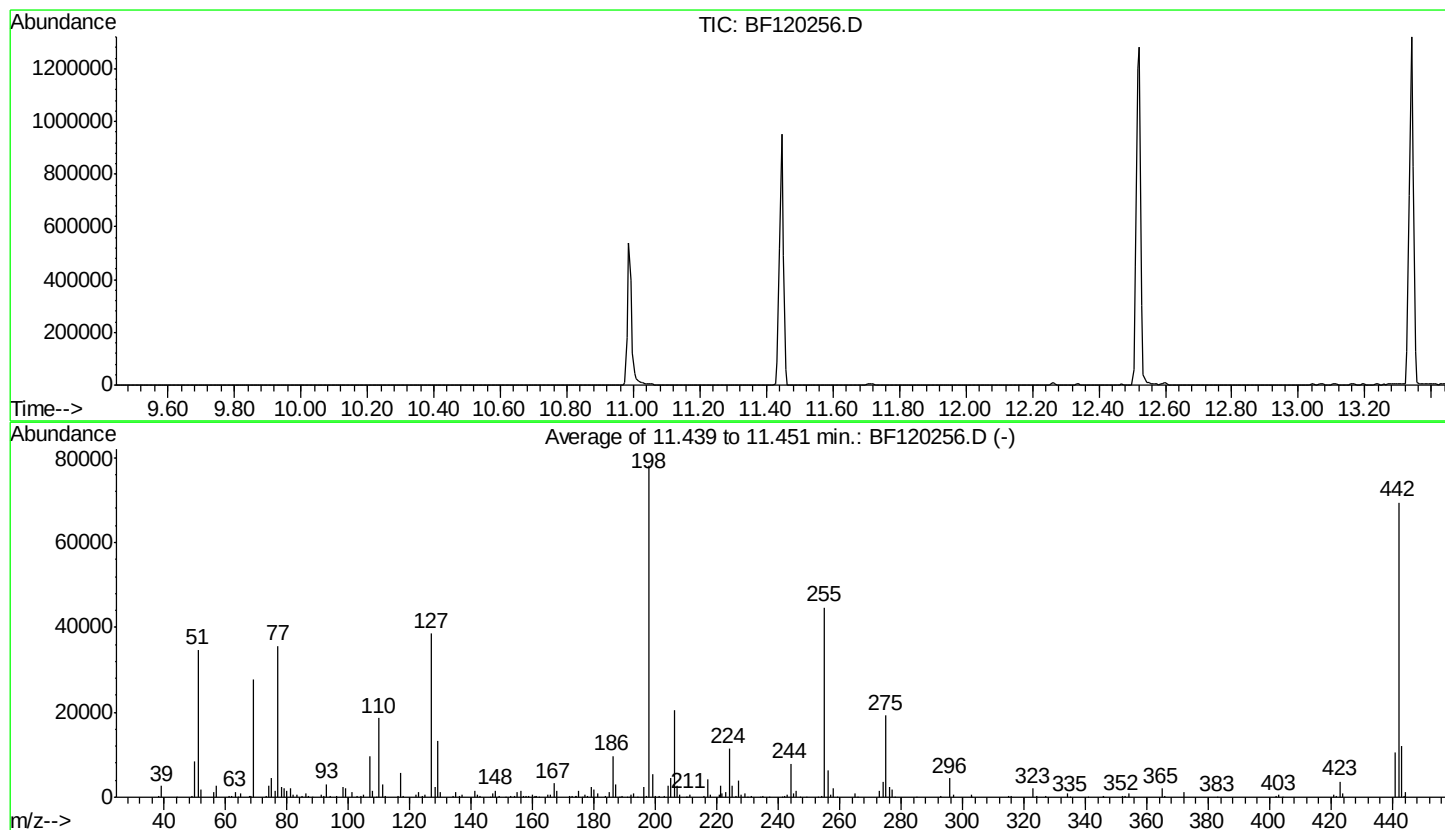

AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	34701	PASS
68	69	0.00	2	1.2	330	PASS
69	198	0.00	100	35.7	27872	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	38573	PASS
197	198	0.00	2	0.5	353	PASS
198	198	100	100	100.0	78088	PASS
199	198	5	9	7.0	5459	PASS
275	198	10	60	24.6	19244	PASS
365	198	1	100	2.6	2054	PASS
441	198	0.01	100	13.7	10677	PASS
442	198	50	100	88.8	69344	PASS
443	442	15	24	17.6	12194	PASS