
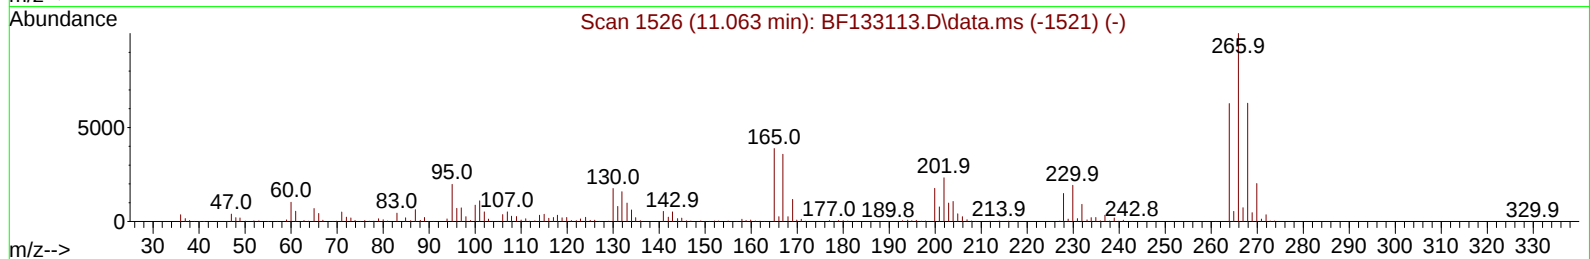
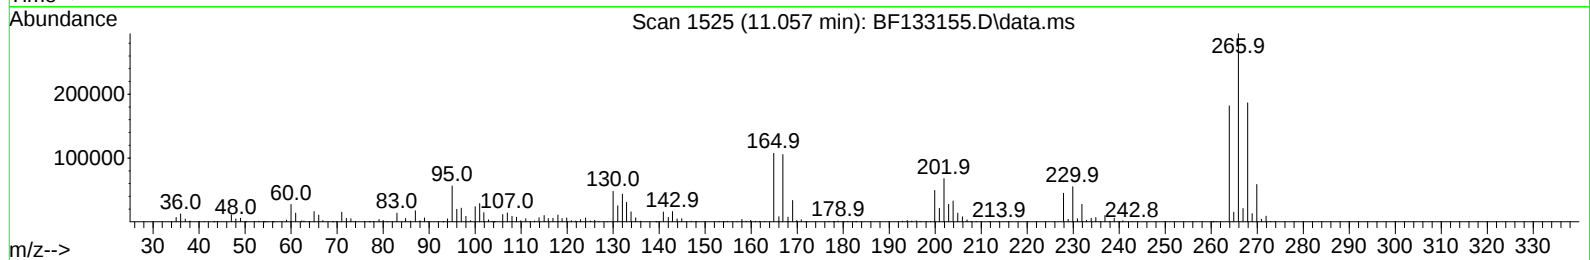


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133155.D
Acq On : 01 May 2023 14:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 15:54:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 15:02:31 2023
Response via : Initial Calibration

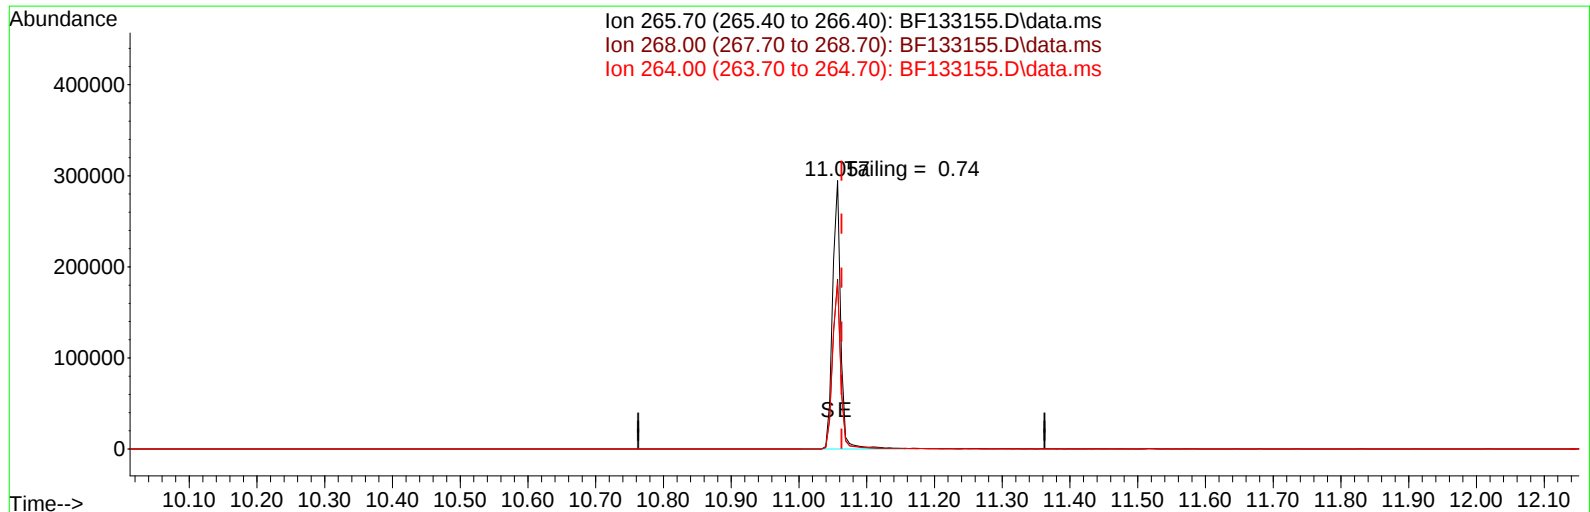

TIC: BF133155.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.006) 98678.11 ng

response 245241

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.26
264.00	63.30	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133155.D
Acq On : 01 May 2023 14:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 15:54:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 15:02:31 2023
Response via : Initial Calibration

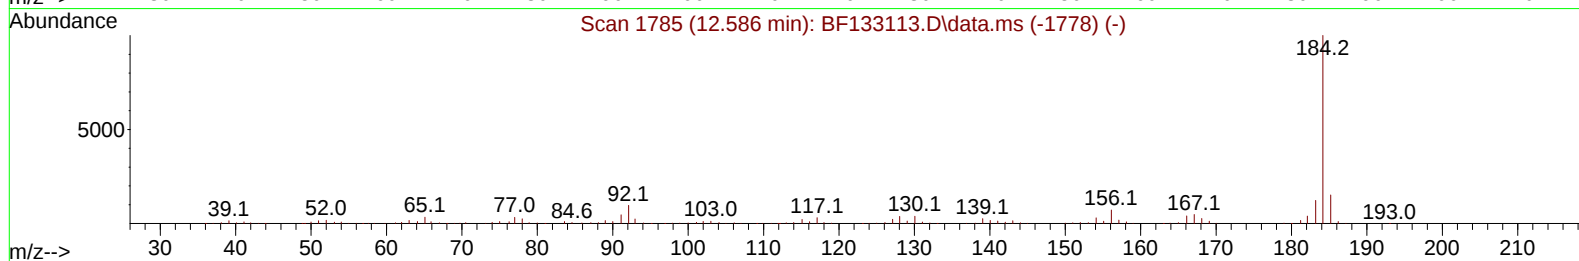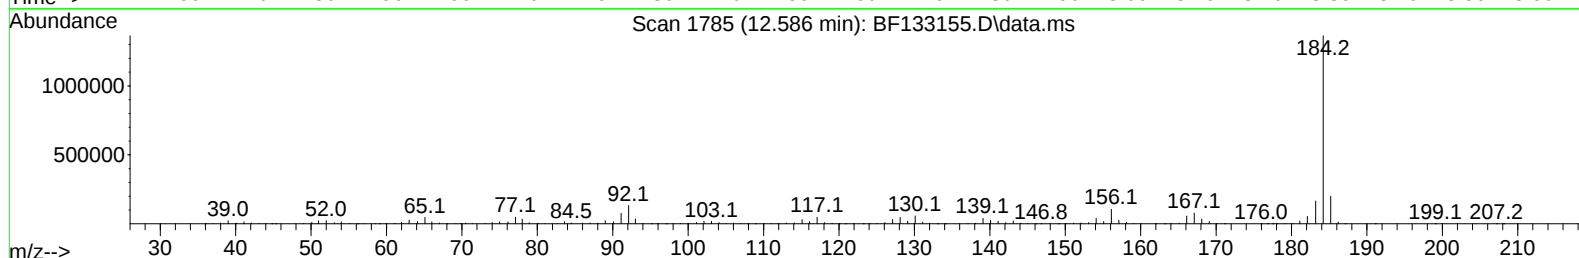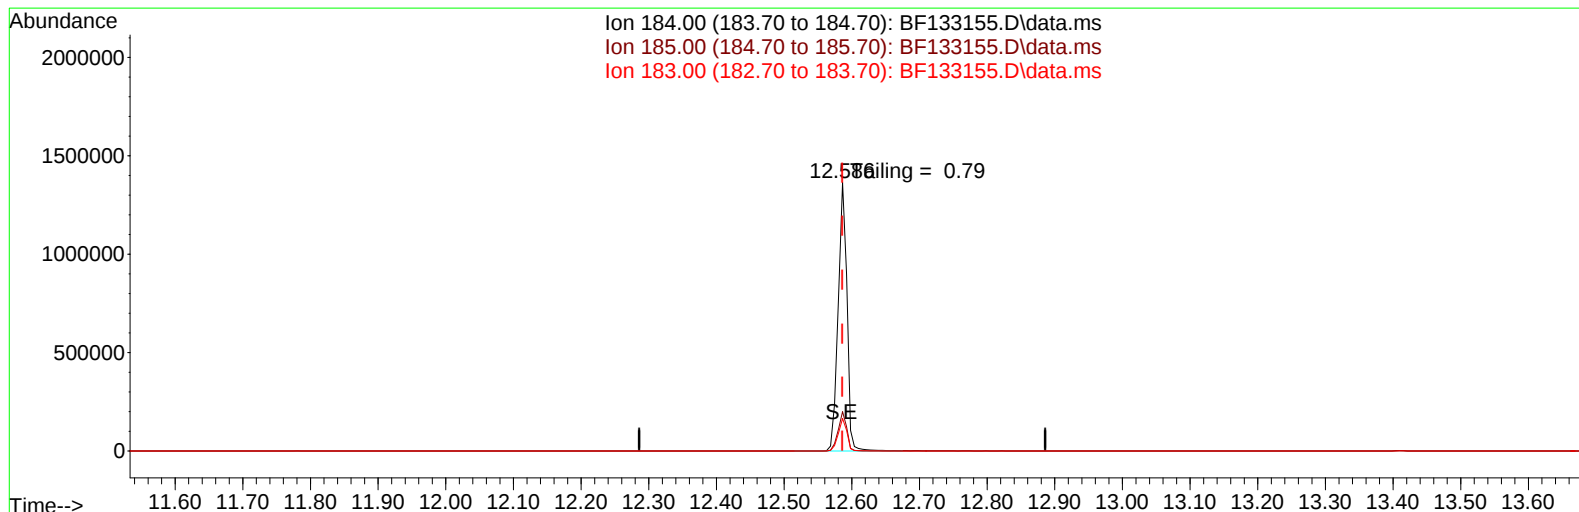

TIC: BF133155.D\data.ms

(77) Benzidine

12.586min (+ 0.000) 131063.03 ng

response 1234504

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.68#
183.00	11.70	12.10
0.00	0.00	0.00