

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
 Data File : BF133162.D
 Acq On : 01 May 2023 18:37
 Operator : CG\JU
 Sample : 02558-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS013-0612-01

Quant Time: May 02 05:21:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 01 15:02:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.728	152	207930	20.000	ng	0.00
21) Naphthalene-d8	8.010	136	855132	20.000	ng	0.00
39) Acenaphthene-d10	9.763	164	448967	20.000	ng	0.00
64) Phenanthrene-d10	11.245	188	798533	20.000	ng	0.00
76) Chrysene-d12	13.880	240	409706	20.000	ng	-0.01
86) Perylene-d12	15.298	264	402477	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	1081136	78.544	ng	0.00
7) Phenol-d6	6.369	99	1364956	79.893	ng	0.00
23) Nitrobenzene-d5	7.293	82	836353	52.792	ng	-0.01
42) 2,4,6-Tribromophenol	10.551	330	318557	70.552	ng	-0.01
45) 2-Fluorobiphenyl	9.092	172	1463868	54.549	ng	0.00
79) Terphenyl-d14	12.833	244	1524494	64.174	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133162.D
Acq On : 01 May 2023 18:37
Operator : CG\JU
Sample : 02558-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS013-0612-01


Quant Time: May 02 05:21:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 15:02:31 2023
Response via : Initial Calibration

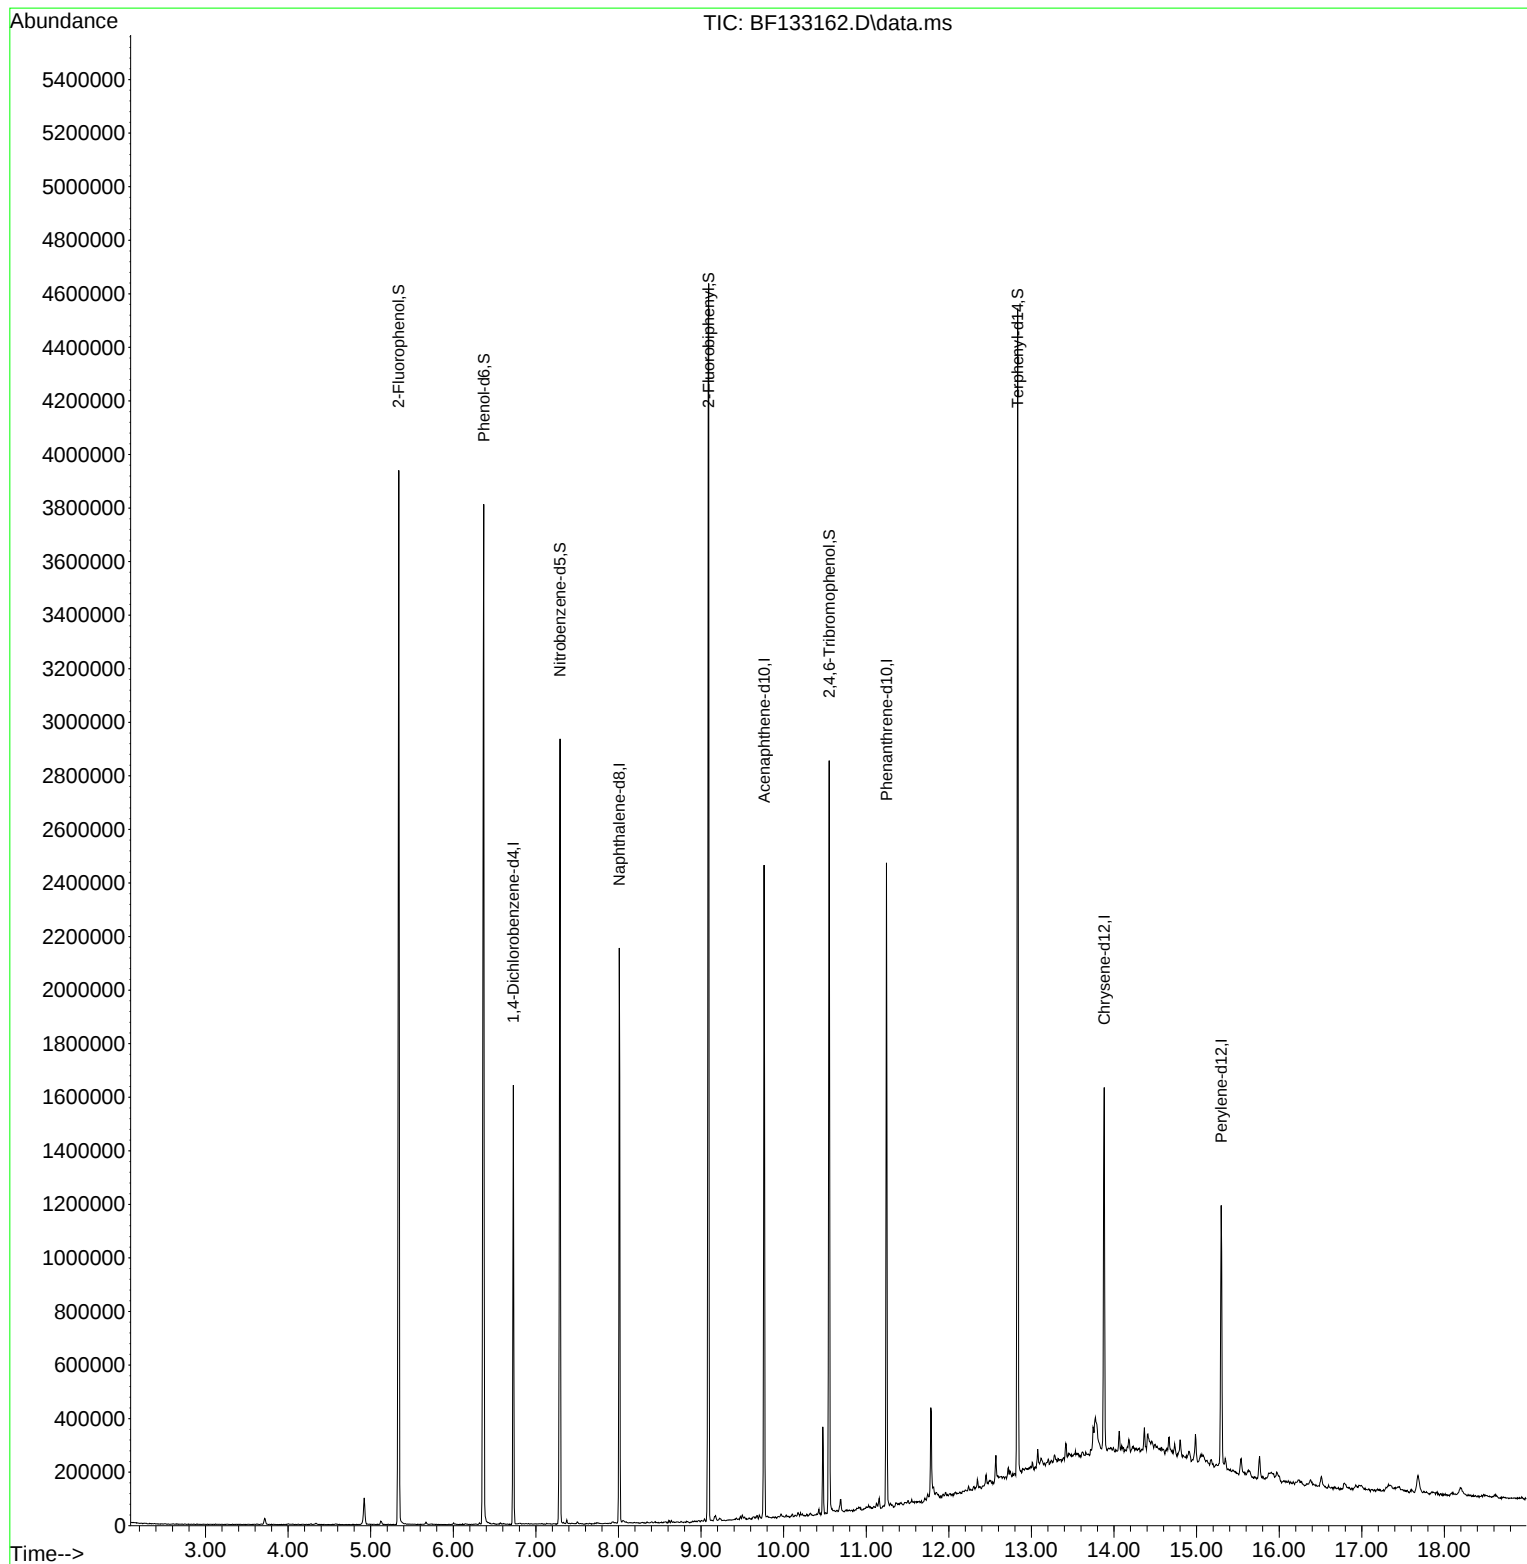






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.728 min Scan# 791
Delta R.T. -0.005 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37

Instrument :
BNA_F
ClientSampleId :
P001-SS013-0612-01



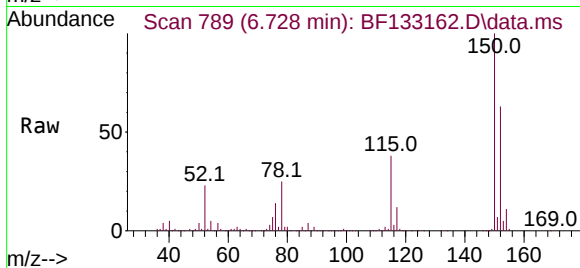



Tgt Ion:152 Resp: 207930
Ion Ratio Lower Upper
152 100
150 158.7 124.8 187.2
115 60.5 49.9 74.9

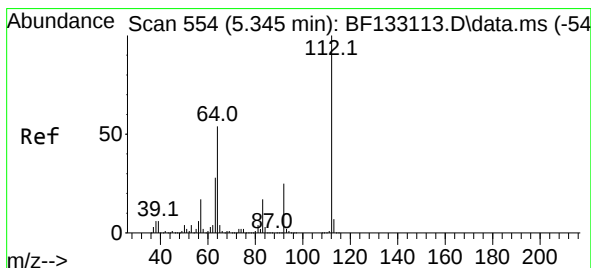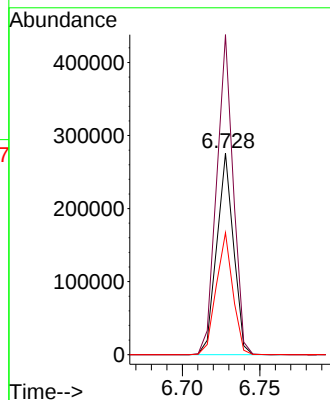

#5
2-Fluorophenol
Concen: 78.544 ng
RT: 5.340 min Scan# 553
Delta R.T. 0.000 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37


Tgt Ion:112 Resp: 1081136
Ion Ratio Lower Upper
112 100
64 57.2 46.8 70.2
63 29.5 23.8 35.8

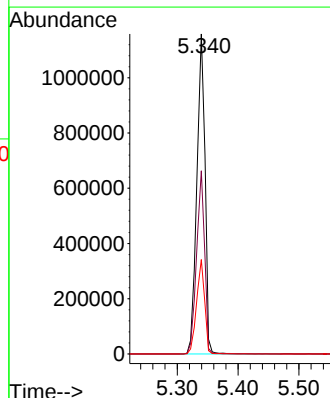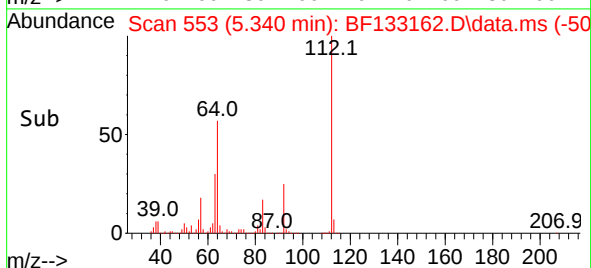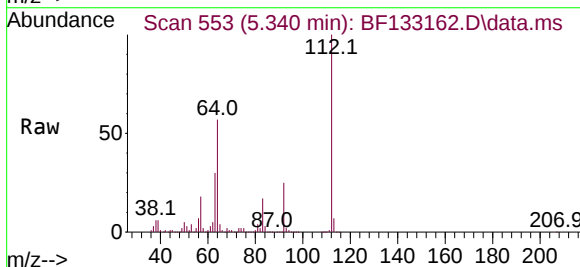






#7
Phenol-d6
Concen: 79.893 ng
RT: 6.369 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37

Instrument :
BNA_F
ClientSampleId :
P001-SS013-0612-01



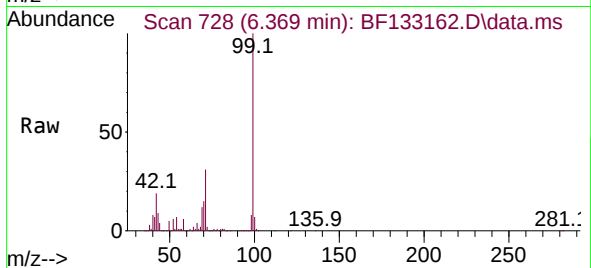



Tgt Ion: 99 Resp: 1364956
Ion Ratio Lower Upper
99 100
42 18.9 16.3 24.5
71 31.5 25.6 38.4

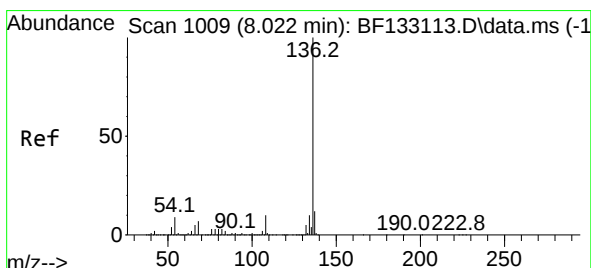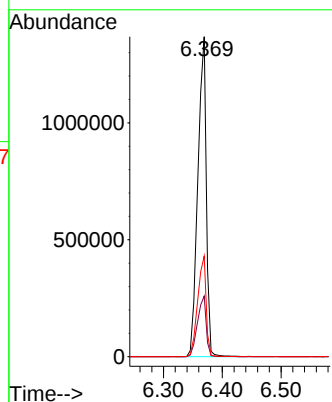

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.010 min Scan# 1007
Delta R.T. -0.006 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37

Tgt Ion: 136 Resp: 855132
Ion Ratio Lower Upper
136 100
137 11.3 8.6 13.0
54 9.0 7.0 10.4
68 7.5 5.4 8.2


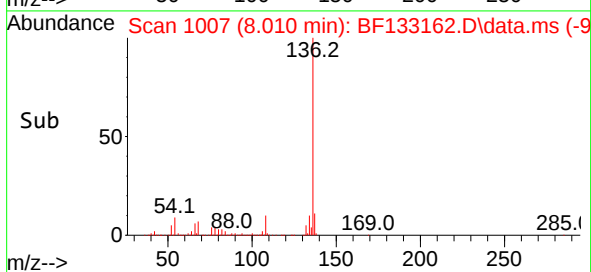
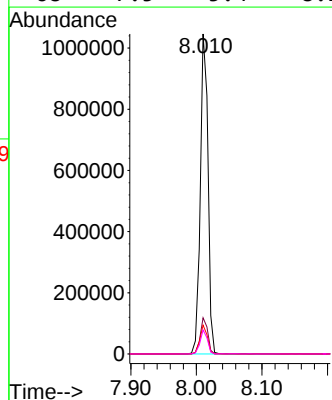



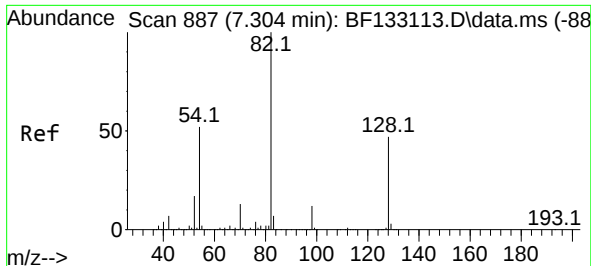

#23
Nitrobenzene-d5
Concen: 52.792 ng
RT: 7.293 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37




Instrument :
BNA_F
ClientSampleId :
P001-SS013-0612-01


Tgt Ion: 82 Resp: 836353
Ion Ratio Lower Upper
82 100
128 48.0 37.7 56.5
54 53.3 43.0 64.4

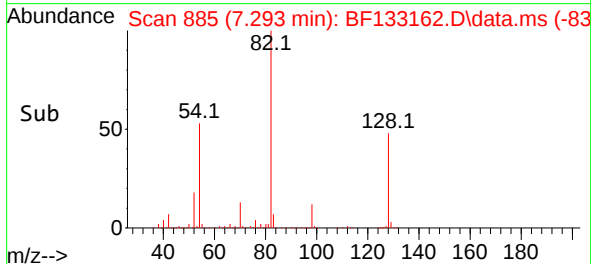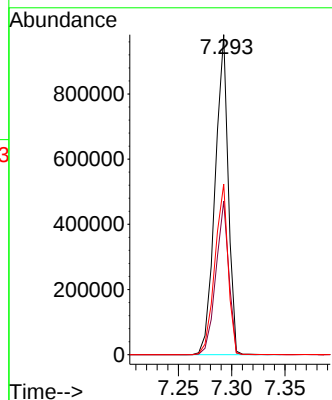

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.763 min Scan# 1305
Delta R.T. -0.006 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37

Tgt Ion:164 Resp: 448967
Ion Ratio Lower Upper
164 100
162 100.0 78.7 118.1
160 43.1 35.8 53.6


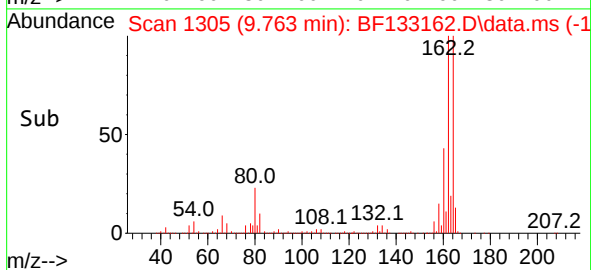
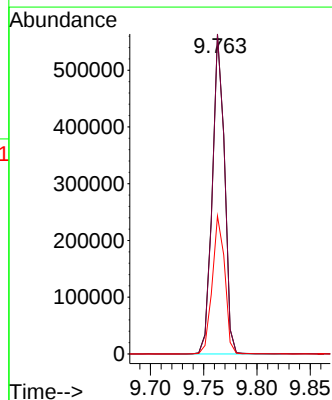
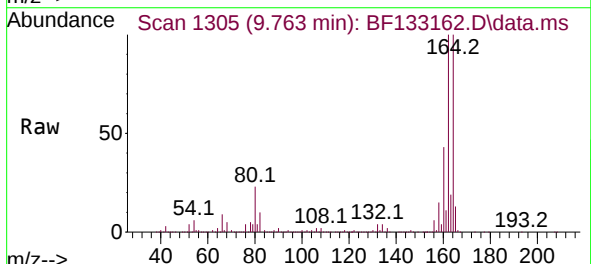


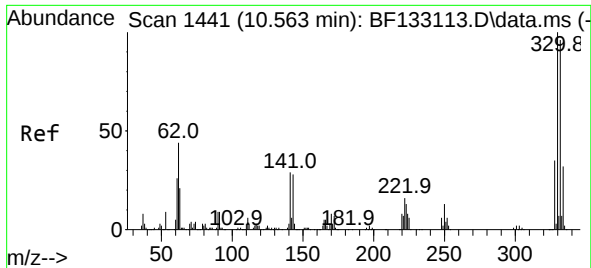

#42
2,4,6-Tribromophenol
Concen: 70.552 ng
RT: 10.551 min Scan# 1441
Delta R.T. -0.012 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37




Instrument :
BNA_F
ClientSampleId :
P001-SS013-0612-01


Tgt Ion:330 Resp: 318557
Ion Ratio Lower Upper
330 100
332 97.7 77.1 115.7
141 32.5 25.8 38.8

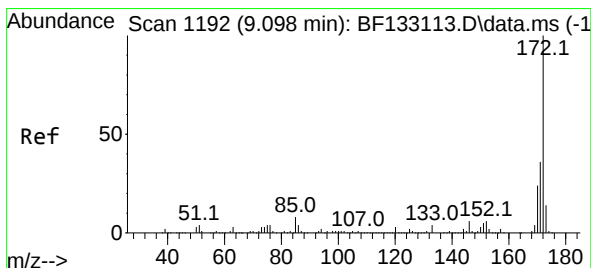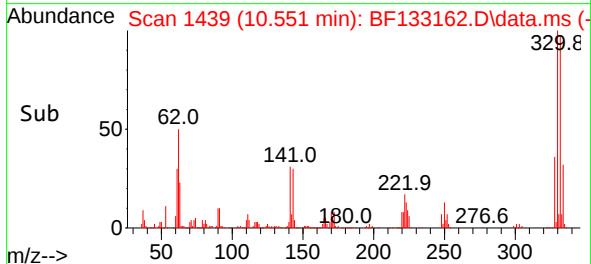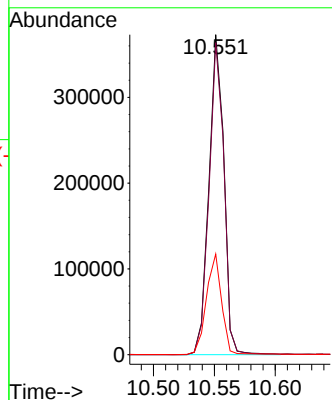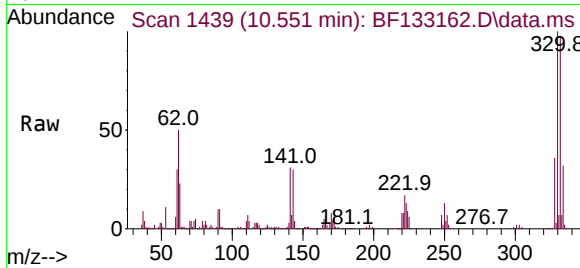

#45
2-Fluorobiphenyl
Concen: 54.549 ng
RT: 9.092 min Scan# 1191
Delta R.T. -0.006 min
Lab File: BF133162.D
Acq: 01 May 2023 18:37

Tgt Ion:172 Resp: 1463868
Ion Ratio Lower Upper
172 100
171 35.9 28.8 43.2
170 24.0 19.4 29.2

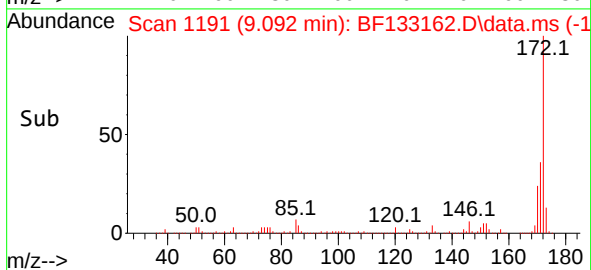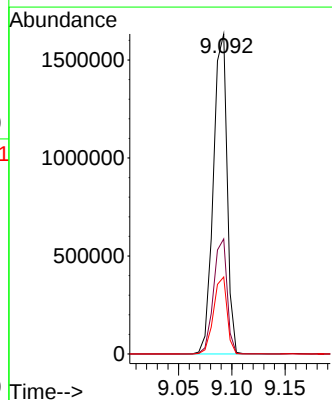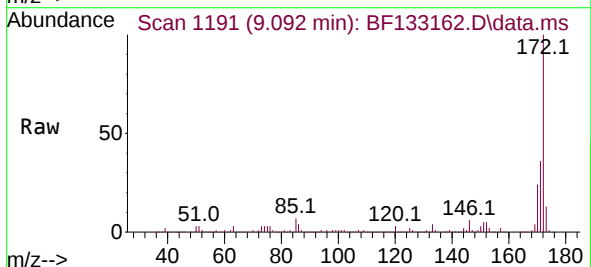

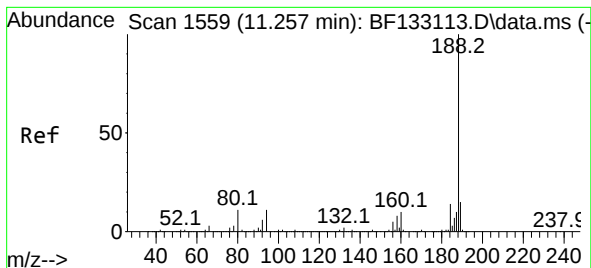

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.245 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF133162.D

Acq: 01 May 2023 18:37

Instrument :

BNA_F

ClientSampleId :

P001-SS013-0612-01





Tgt Ion:188 Resp: 798533

Ion Ratio Lower Upper

188 100

94 11.3 9.7 14.5

80 12.1 10.4 15.6

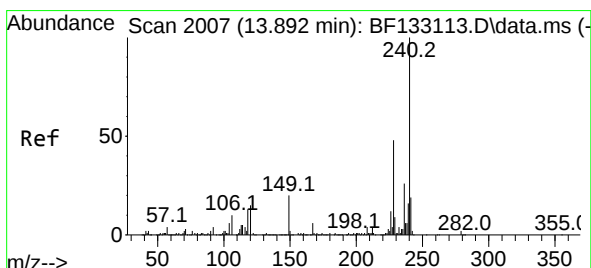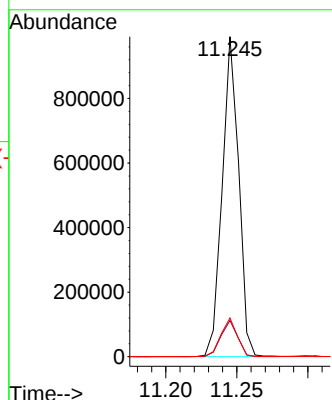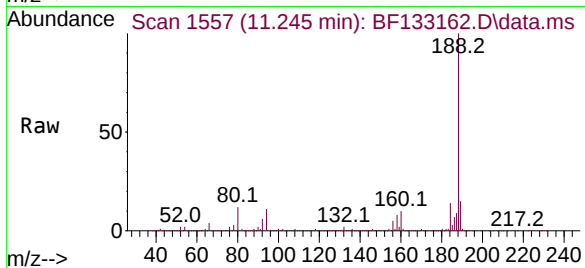

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.880 min Scan# 2005

Delta R.T. -0.012 min

Lab File: BF133162.D

Acq: 01 May 2023 18:37




Tgt Ion:240 Resp: 409706


Ion Ratio Lower Upper

240 100

120 13.1 10.5 15.7

236 26.1 21.5 32.3


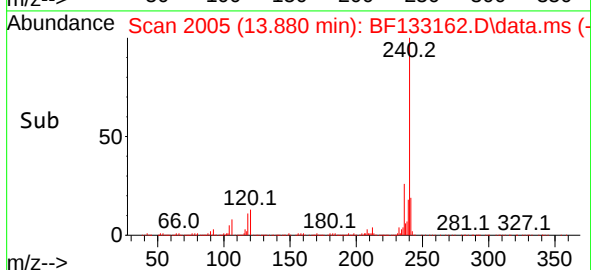
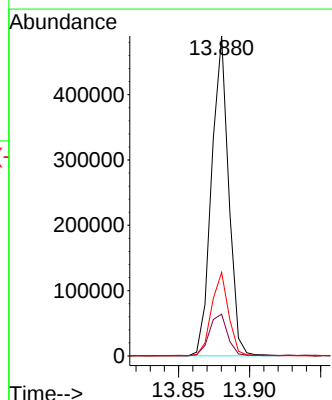
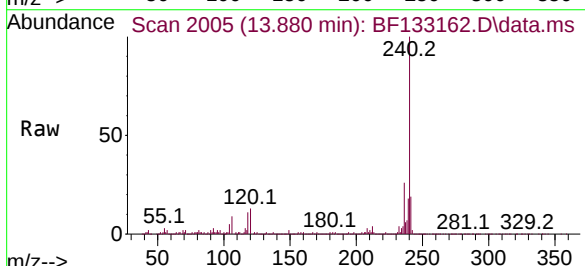




#79
 Terphenyl-d14
 Concen: 64.174 ng
 RT: 12.833 min Scan# 1829
 Delta R.T. -0.006 min
 Lab File: BF133162.D
 Acq: 01 May 2023 18:37

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS013-0612-01

Tgt Ion:244 Resp: 1524494
 Ion Ratio Lower Upper
 244 100
 212 6.4 5.1 7.7
 122 12.8 8.6 13.0

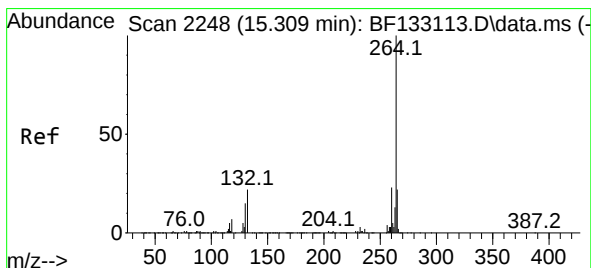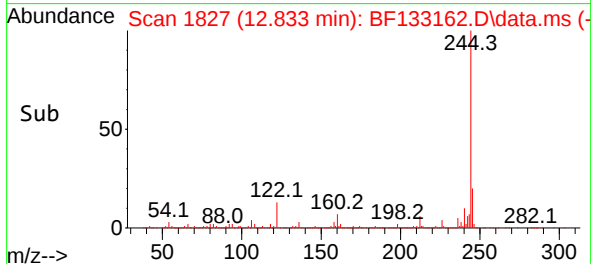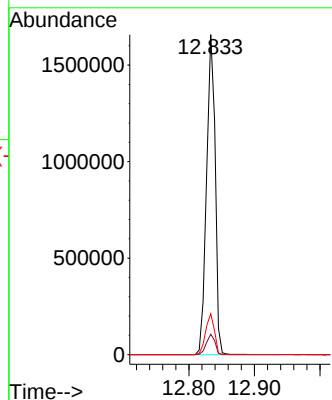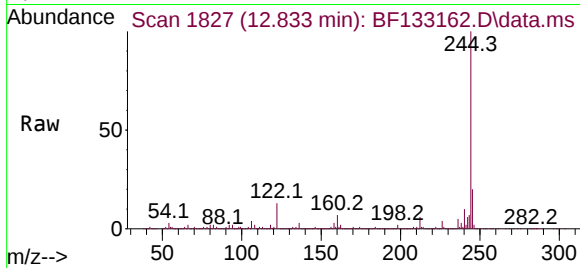

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.298 min Scan# 2246
 Delta R.T. -0.006 min
 Lab File: BF133162.D
 Acq: 01 May 2023 18:37

Tgt Ion:264 Resp: 402477
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.8 28.2
 265 21.6 17.0 25.4

