

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
 Data File : BF133161.D
 Acq On : 01 May 2023 18:06
 Operator : CG\JU
 Sample : 02521-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	477	480	488	rVB	56509	73481	1.11%	0.224%
2	5.340	548	553	556	rBV	2668781	2601988	39.19%	7.922%
3	6.363	723	727	730	rBV	1974431	1624147	24.47%	4.945%
4	6.728	785	789	792	rBV	1451910	1095963	16.51%	3.337%
5	7.298	880	886	888	rBV	3687507	3772610	56.83%	11.485%
6	8.010	1004	1007	1011	rBV	1830286	1492379	22.48%	4.543%
7	9.092	1186	1191	1194	rBV	6808692	6165704	92.88%	18.771%
8	9.763	1301	1305	1309	rBV	2199486	1712242	25.79%	5.213%
9	10.557	1435	1440	1443	rBV	3764335	3768892	56.77%	11.474%
10	11.245	1553	1557	1560	rBV	2195566	1758419	26.49%	5.353%
11	12.839	1823	1828	1831	rBV	6160034	6638653	100.00%	20.211%
12	13.880	2001	2005	2009	rBV	1254467	1121141	16.89%	3.413%
13	15.298	2241	2246	2251	rBV	878419	1021350	15.38%	3.109%




Sum of corrected areas: 32846969

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133161.D
Acq On : 01 May 2023 18:06
Operator : CG\JU
Sample : 02521-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

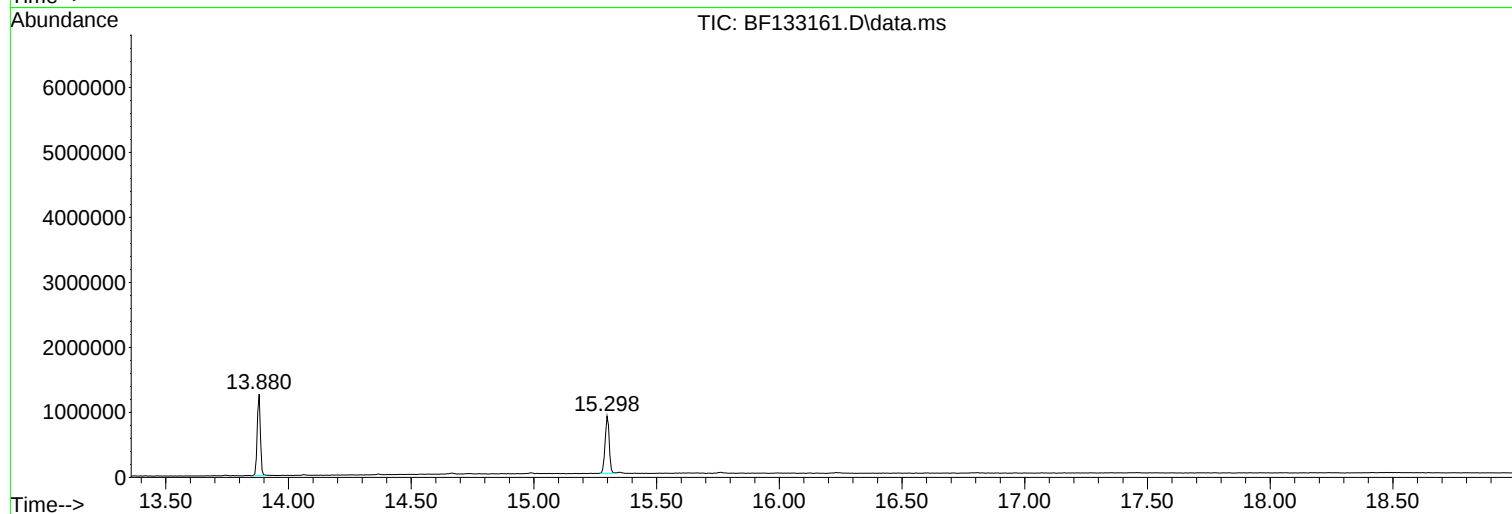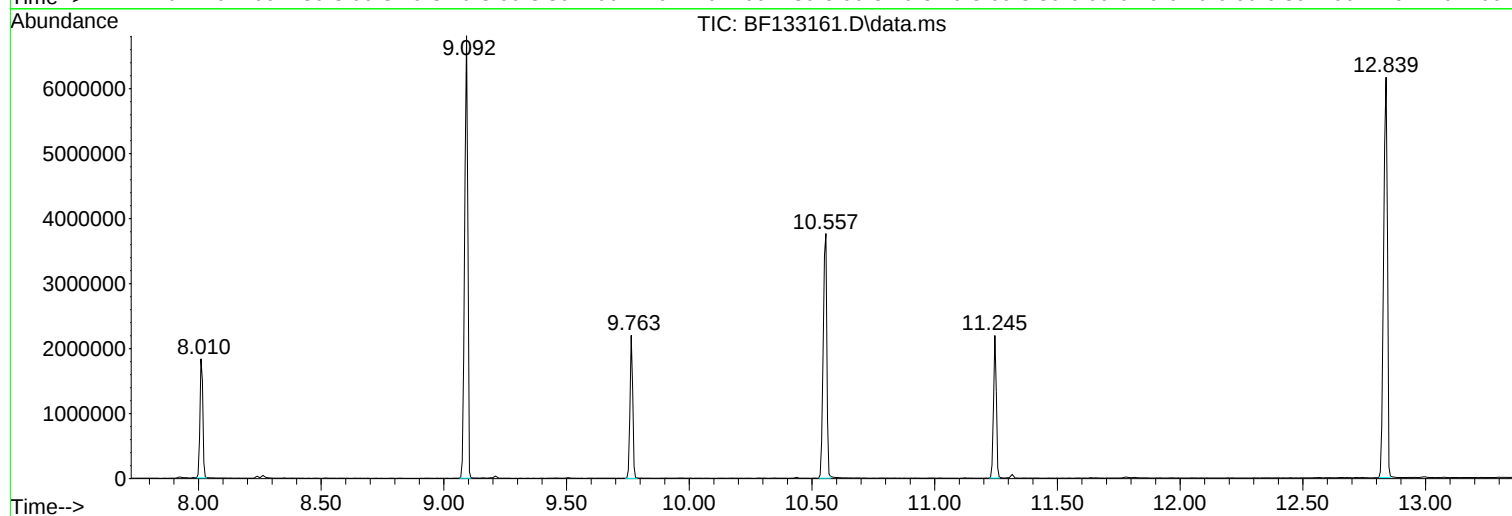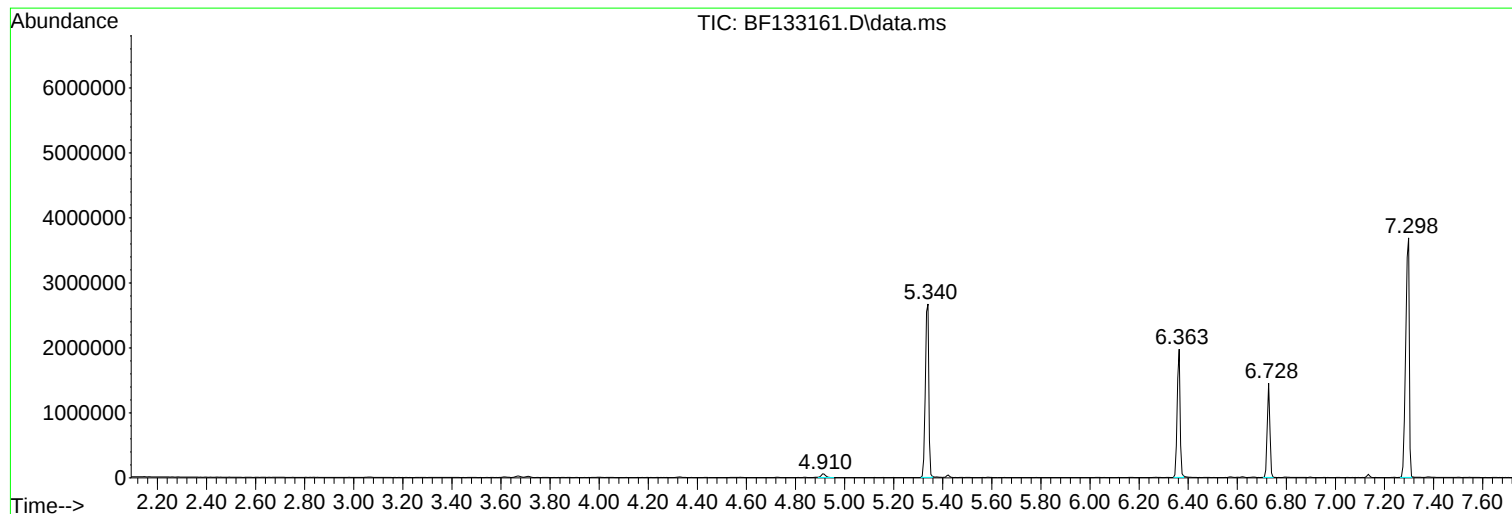

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133161.D
Acq On : 01 May 2023 18:06
Operator : CG\JU
Sample : 02521-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133161.D
Acq On : 01 May 2023 18:06
Operator : CG\JU
Sample : 02521-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------