
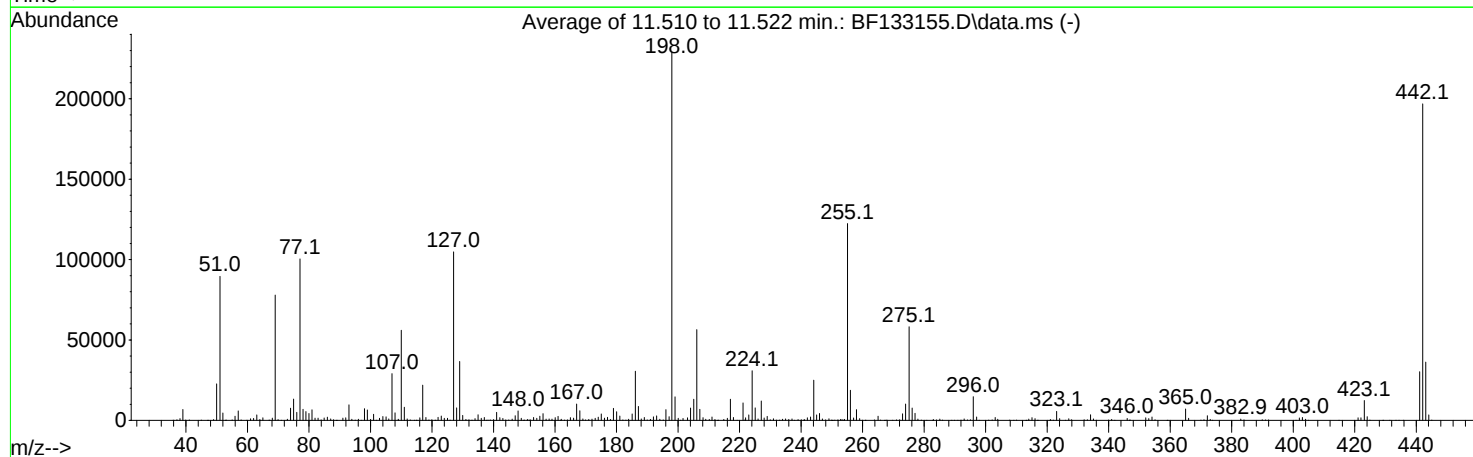


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133155.D
Acq On : 01 May 2023 14:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 02 10:52:52 2023

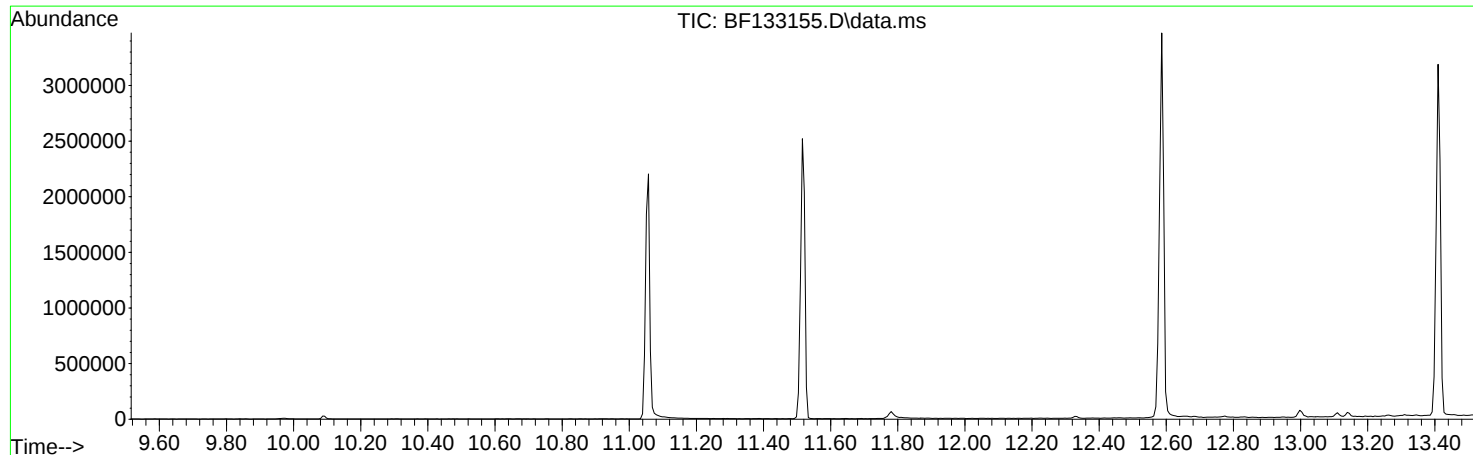

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	89596	PASS
68	69	0.00	2	1.8	1379	PASS
69	198	0.00	100	34.1	77926	PASS
70	69	0.00	2	0.6	465	PASS
127	198	10	80	45.8	104837	PASS
197	198	0.00	2	1.0	2326	PASS
198	198	100	100	100.0	228779	PASS
199	198	5	9	6.4	14663	PASS
275	198	10	60	25.4	58224	PASS
365	198	1	100	3.1	7080	PASS
441	198	0.01	100	13.2	30241	PASS
442	442	50	100	100.0	196835	PASS
443	442	15	24	18.4	36211	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/1/2023	BNA_F	<u>BF133155.D</u>
Compound Name	Response	Retention Time
DDT	546492	13.41
DDD	10780	13.11
DDE	1571	12.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12351	558843	2.21

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
 Data File : BF133155.D
 Acq On : 01 May 2023 14:54
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 01 15:54:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 01 15:02:31 2023
 Response via : Initial Calibration

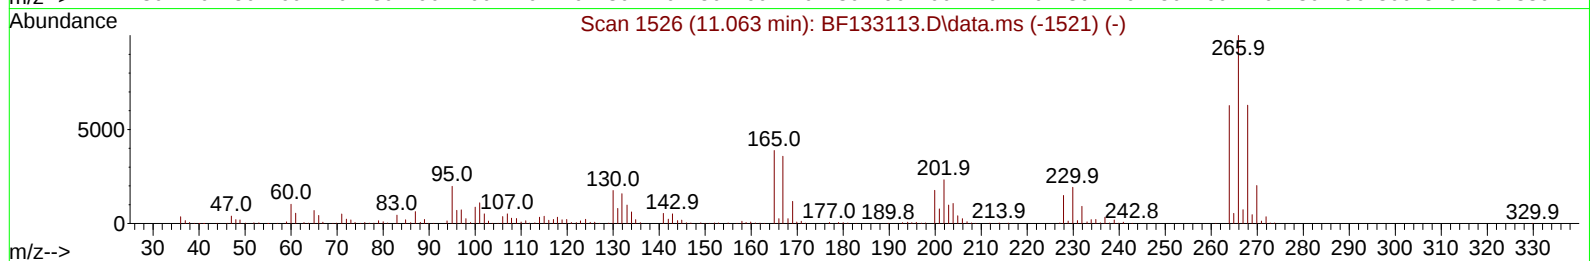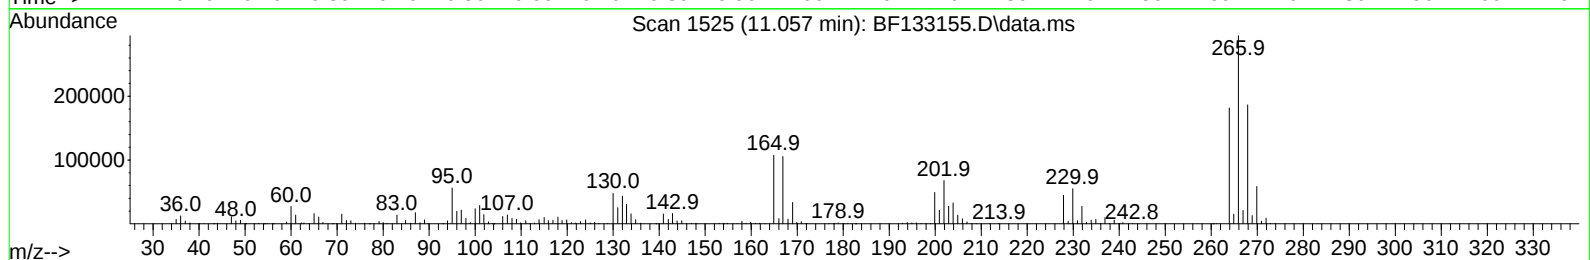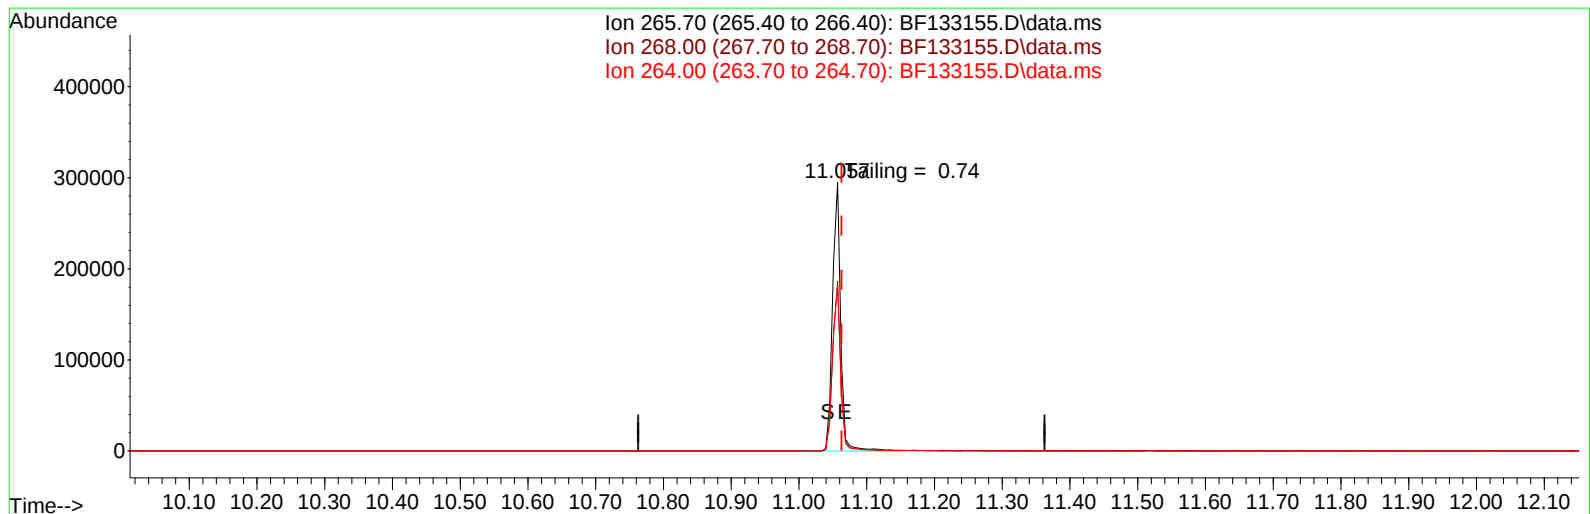

TIC: BF133155.D\data.ms

(70) Pentachlorophenol (C)

11.057min (-0.006) 98678.11 ng




response 245241

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.26
264.00	63.30	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050123\
Data File : BF133155.D
Acq On : 01 May 2023 14:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 01 15:54:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 15:02:31 2023
Response via : Initial Calibration

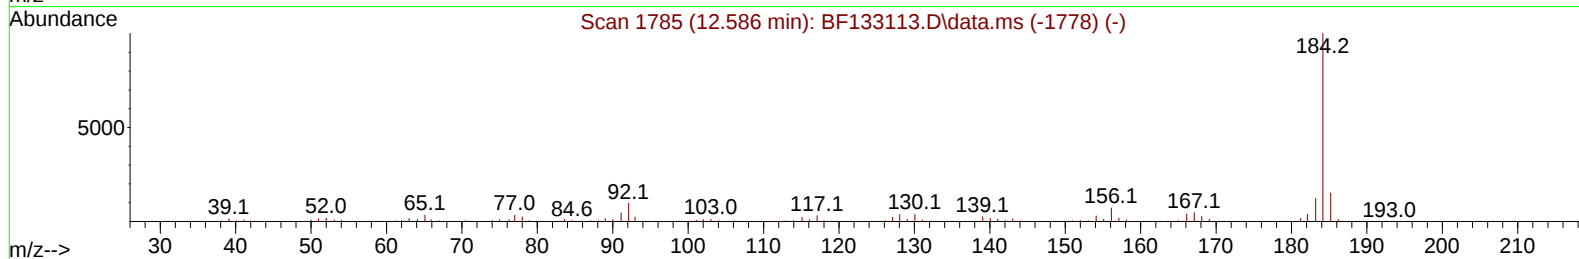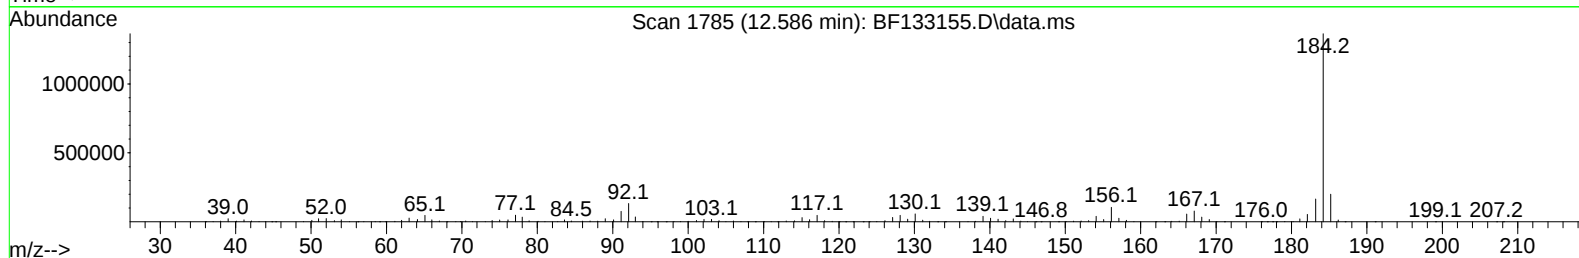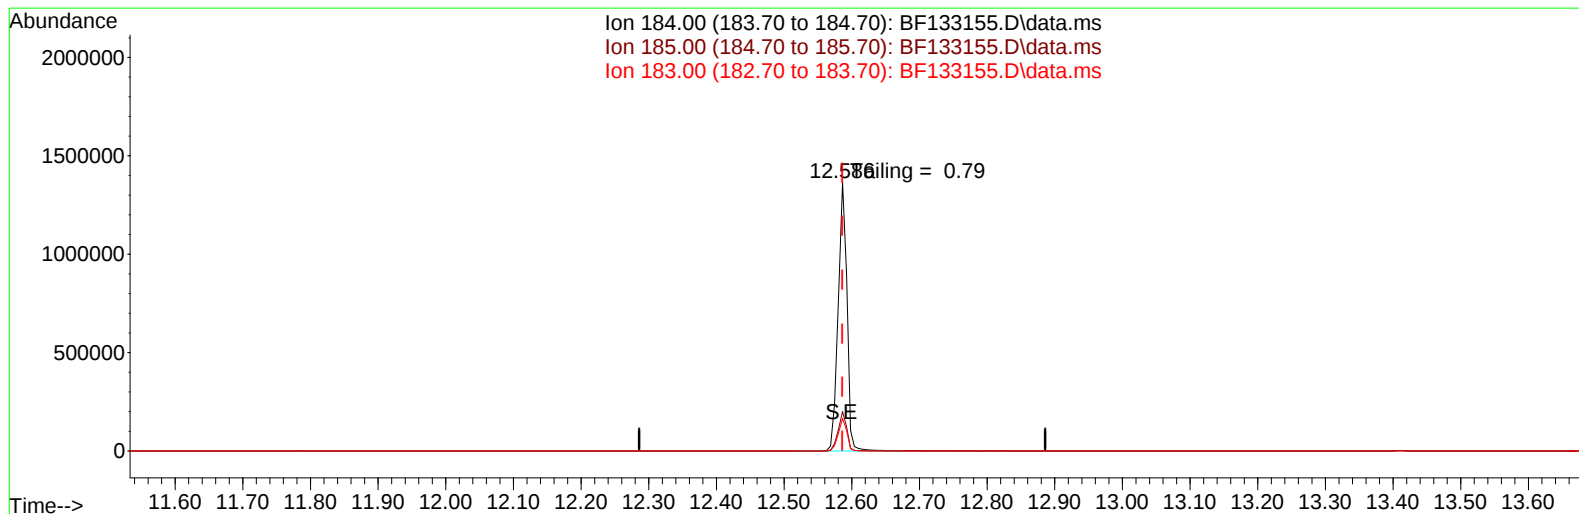

TIC: BF133155.D\data.ms

(77) Benzidine

12.586min (+ 0.000) 131063.03 ng

response 1234504

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.68#
183.00	11.70	12.10
0.00	0.00	0.00