


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050324\
Data File : BF137826.D
Acq On : 03 May 2024 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

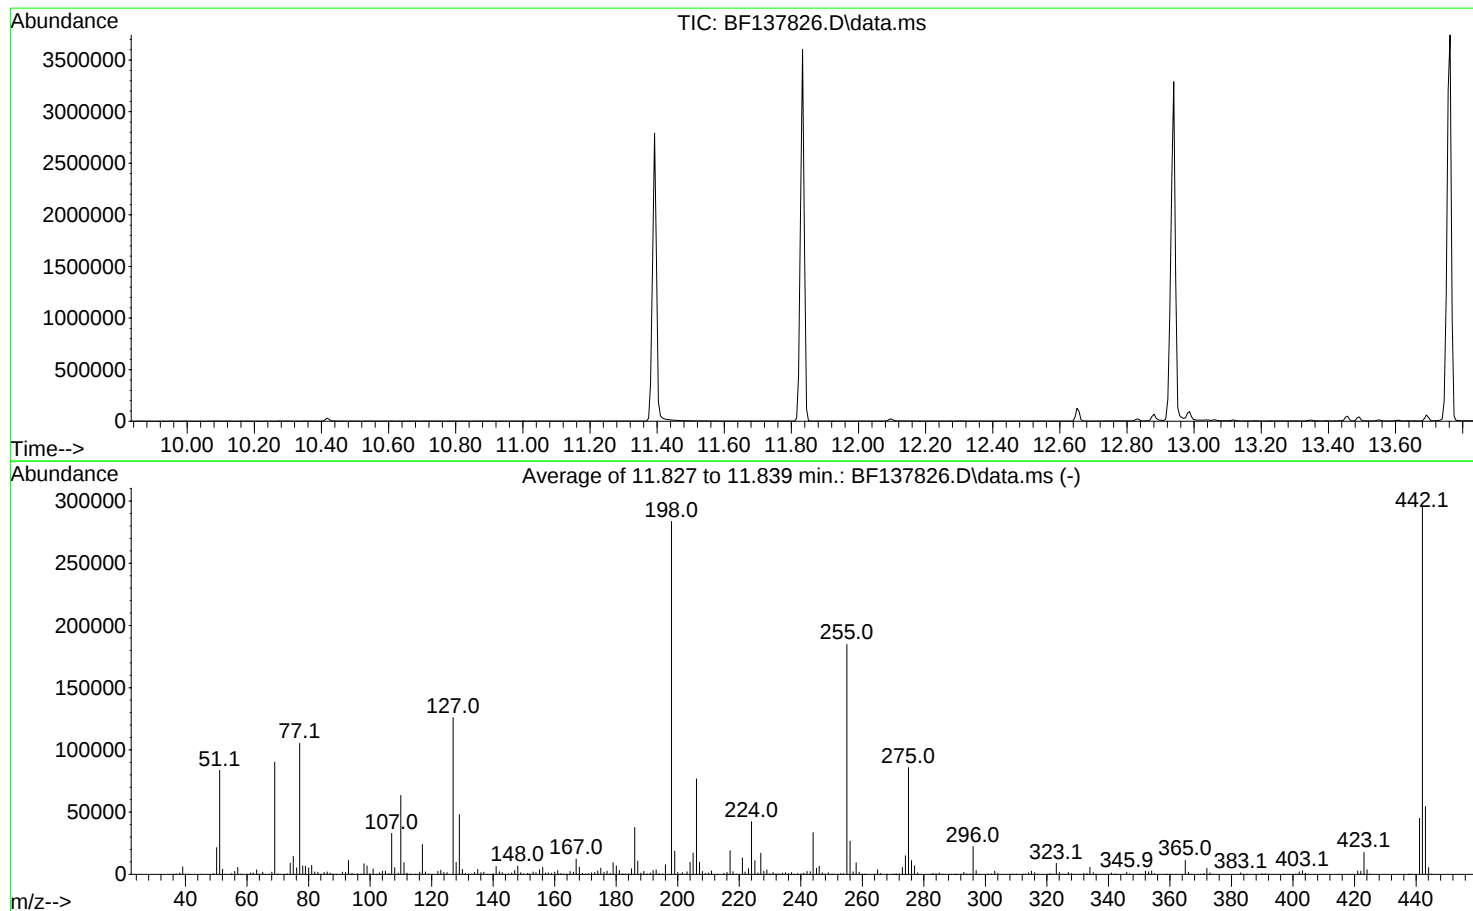

AutoFind: Scans 1656, 1657, 1658; Background Corrected with Scan 1650

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	83571	PASS
68	69	0.00	2	2.0	1791	PASS
69	198	0.00	100	31.8	90120	PASS
70	69	0.00	2	0.6	523	PASS
127	198	10	80	44.4	126016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	283669	PASS
199	198	5	9	6.6	18642	PASS
275	198	10	60	30.2	85795	PASS
365	198	1	100	4.0	11350	PASS
441	198	0.01	100	15.9	44963	PASS
442	442	50	100	100.0	295659	PASS
443	442	15	24	18.5	54563	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/3/2024	BNA_F	<u>BF137826.D</u>
Compound Name	Response	Retention Time
DDT	680958	13.762
DDD	15192	13.457
DDE	1530	13.116
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16722	697680	2.40

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050324\
Data File : BF137826.D
Acq On : 03 May 2024 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 03 13:47:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

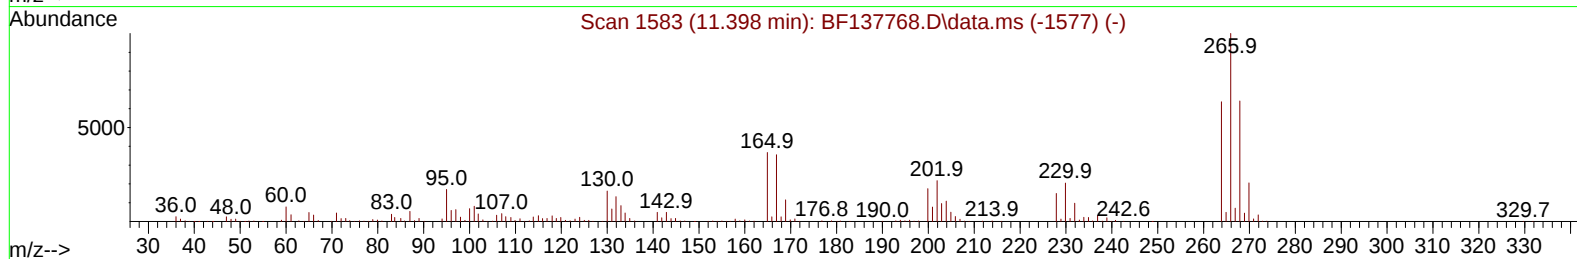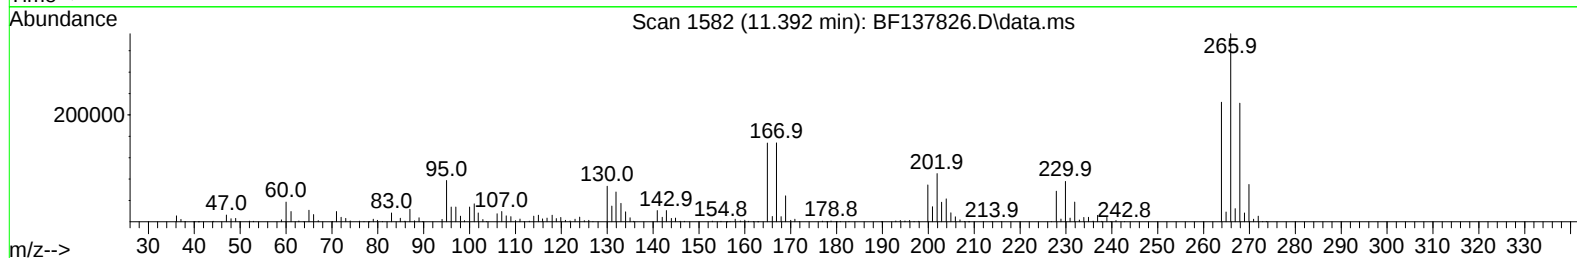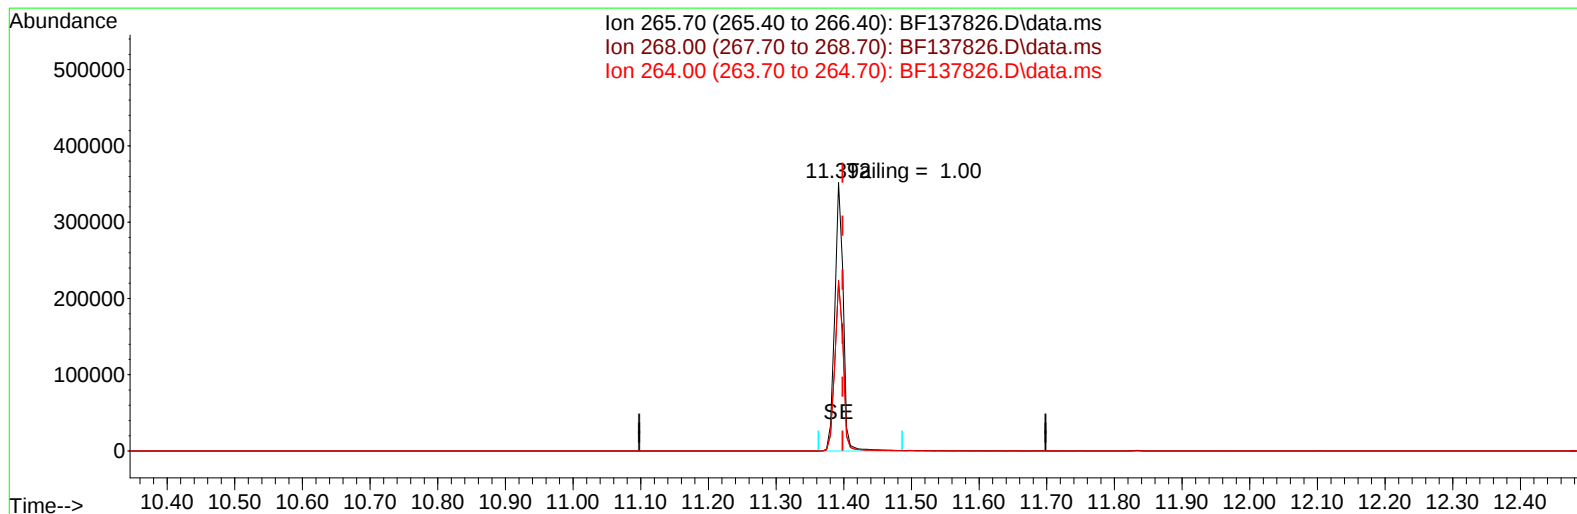

TIC: BF137826.D\data.ms

(70) Pentachlorophenol (C)

11.392min (-0.006) 613128.49 ng




response 305230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.05
264.00	63.70	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050324\
Data File : BF137826.D
Acq On : 03 May 2024 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 03 13:47:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

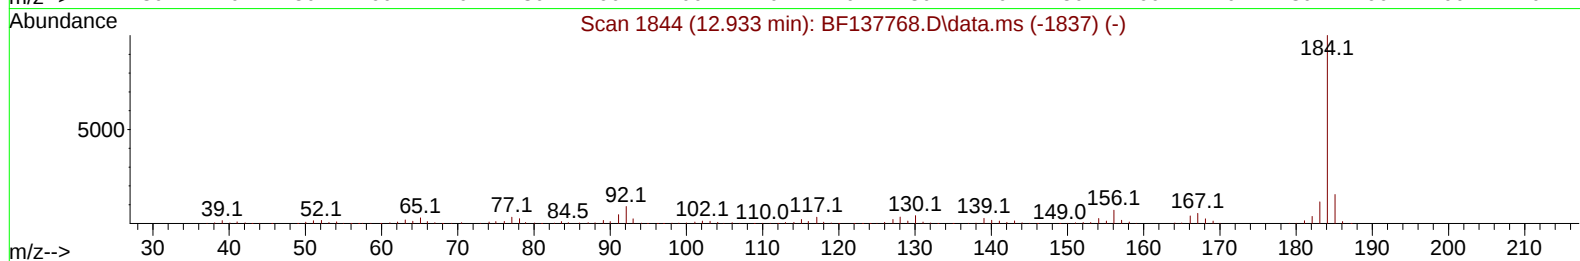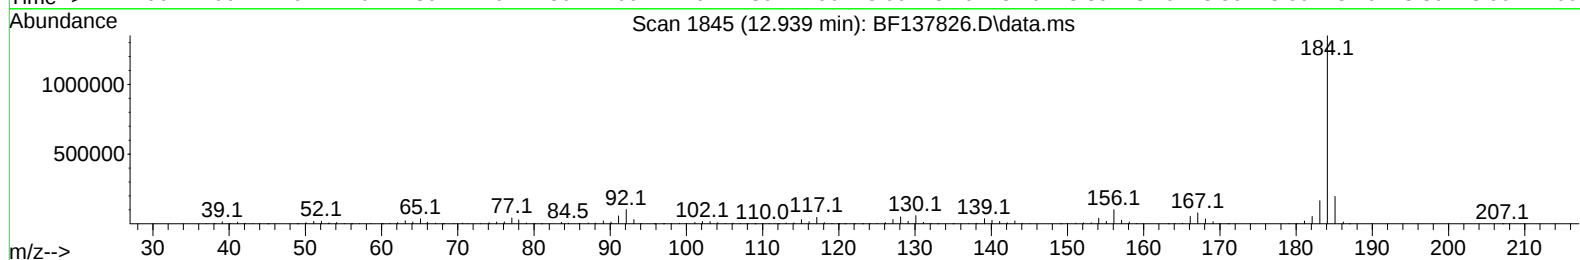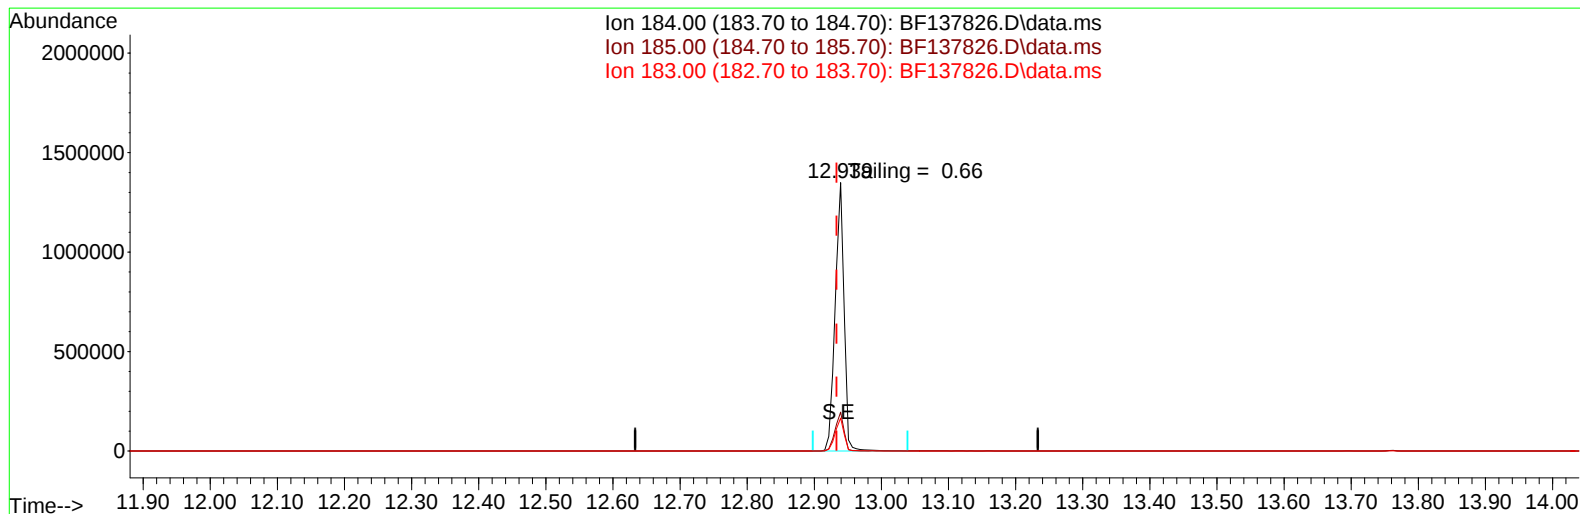

TIC: BF137826.D\data.ms

(77) Benzidine

12.939min (+ 0.006) 0.00 ng

response 1240818

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.53
183.00	11.50	12.29
0.00	0.00	0.00