
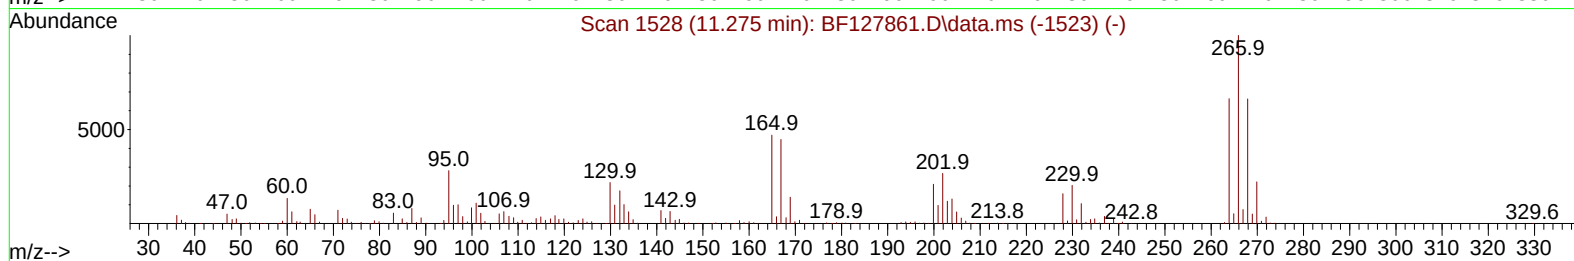
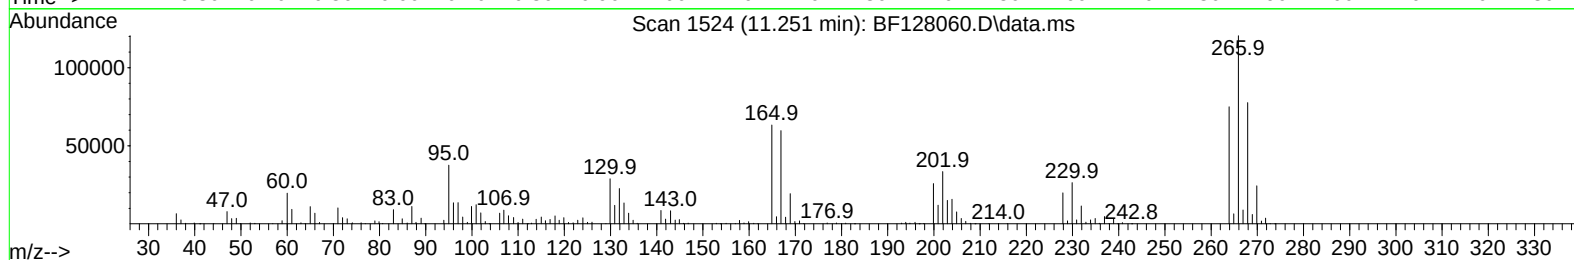


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
Data File : BF128060.D
Acq On : 04 May 2022 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 13:48:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 04:23:29 2022
Response via : Initial Calibration

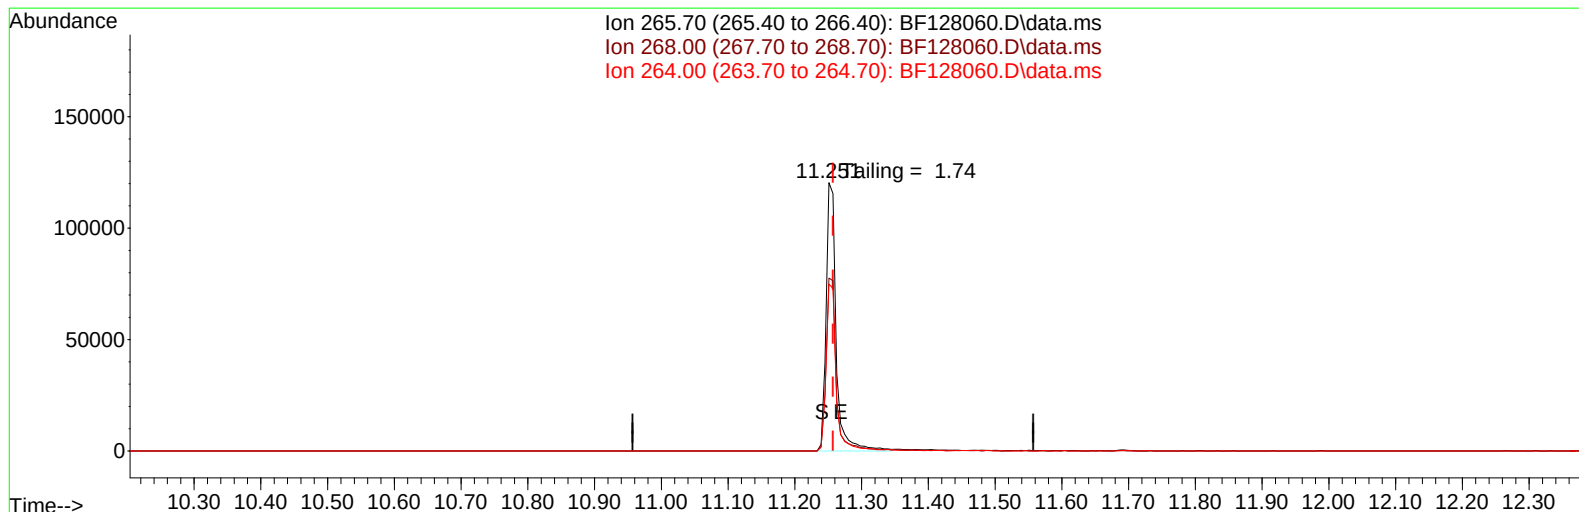

TIC: BF128060.D\data.ms

(70) Pentachlorophenol (C)




11.251min (-0.006) 22274.88 ng

response 127341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.48
264.00	66.40	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050422\
 Data File : BF128060.D
 Acq On : 04 May 2022 09:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 13:48:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 04:23:29 2022
 Response via : Initial Calibration

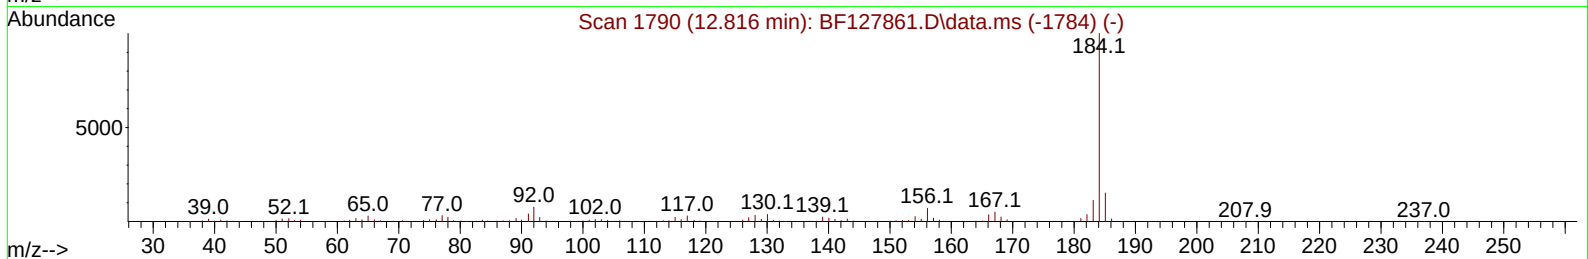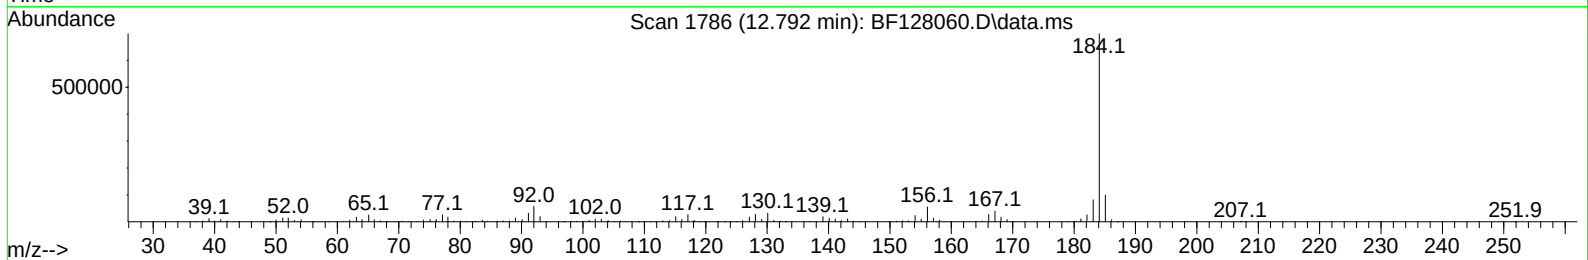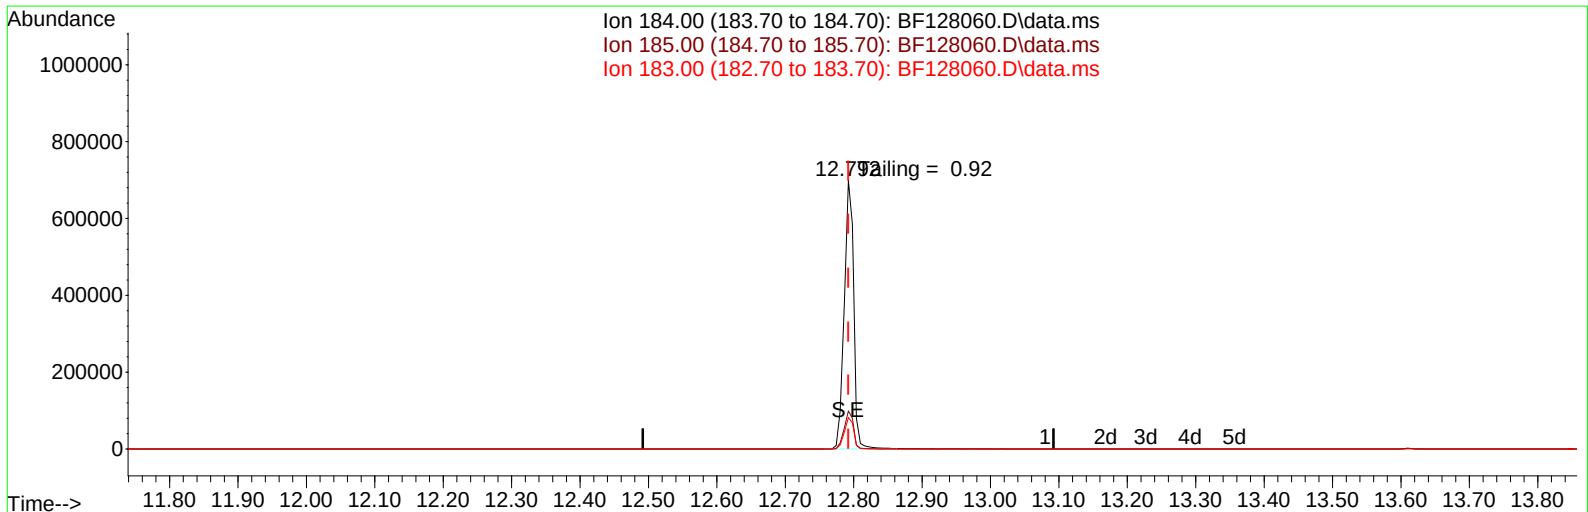

TIC: BF128060.D\data.ms

(77) Benzidine

12.792min (0.000) 546046.42 ng m

response 671579

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.21
183.00	11.20	11.71
0.00	0.00	0.00